







HELMUT

Content

ZEPF IK GMBH

101-01-00





ABI

Company Profile 01-05



Professor Ferdinand Sauerbruch became famous for a special surgical technique that he had developed. As a surgeon, he had rather clear-cut ideas regarding the characteristics and quality of the surgical instruments he used. It was not easy to meet his high standards. The well-known surgeon turned to Zepf, an instrument manufacturer in Seitingen that back then was still a rather young company, to produce the surgical instruments he wanted, as well as special prototype arm and leg prostheses.

Isidor Zepf, who had founded the company in 1921, and his wife Rosa, who was surely one of the first female surgical instrument makers, were able to produce the Berlin professor's products the way he wanted. Their - back in those days - somewhat unusual collaboration built the foundation for Zepf's successful development effort and demonstrated what is even today Zepf's hallmark: rapidly implementing innovations in the field of medical instruments, working in collaboration with well-known physicians and developing these innovations into exemplary solutions. What had been a manufacturing plant with modest beginnings began to grow due to the growing demand for medical instruments.

Helmut Zepf senior and Helmut Zepf junior developed the company in the following decades to a leading manufacturer of dental instruments in Germany.

AESTHETIC IS THE RESULT



⁰¹⁻⁰⁶ Company Profile

49 (0) 74 64 / 98 88 (





Craftmanship since 1921

Today we are still a family company, managed in the fourth generation by Patrick Zepf. Our decisions are still based on the strict maintaining of basic standards and Zepf's quality criteria and high innovation. A family needs a home. The home of the Zepf family of course is Seitingen-Oberflacht where we reside since 1921.

Here we can count on the extensive technical know-how of our employees, many of them proving their loyalty to us for decades, since it is well known that this particular region of Baden-Württemberg is a hotbed of inventiveness and creativity. Last, but not least, Tuttlingen and the surrounding area has managed to remain the center of the world's medical-equipment industry, thanks to its abundance of well-trained skilled workers. It is companies like Helmut Zepf, to mention just one example, that have been standing for that reputation in the field for more than three-quarters of a century.

Consistent with our corporate philosophy, we see ourselves as driver of innovation. In the footsteps of others we cannot improve. We consciously take into account that a development is allowed to fail.

Loyal customers who appreciate our innovations are our reward.

Thank you for your confidence!



0





K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

RELAX

zepf-dental.com

The "New Generation Handles"

The **ZSHAPE** Relax handles were designed according to ergonomic knowledge for the optimal working process during the curettage.

Diagnostic 02-01

The handles are coated with the new **ZEPF** nanget coating. The black-coated **ZEPF** nanget curettes have a durable, very hard surface which is very aggressive and sharp-edged, due to their crystalline nanostructure.

With the unique coating, the surface hardness is increased to an unprecedented **4500 Vickers**.

The black, scratch-resistant surface is easy to clean and prevents unpleasant light reflections.

As usual, the instrument tips are interchangeable due to the M4 x 0.5 mm thread. $\ensuremath{\textit{QUICKFIX}}$

Handle colors
HELMUT ZEPF
Z°SHAPE Relax
handles:
26.010.01OX

	20.010.010X	yellow
	26.010.02OX	brown
	26.010.03OX	violet
	26.010.04OX	signal purple
	26.010.05OX	champagne
	26.010.06OX	turquoise
	26.010.07OX	cobalt-blue
	26.010.08OX	yellow-green
	26.010.09OX	mint
Ш	26.010.10OX	black



02-02 Diagnostic

are mentioned in the index from page 11-07. CC K2019-03/1-E

49 (0) 74 64 / 98 88 0

These handles are light, manufactured from top-quality plastic with a satin surface finish, available in ten colors. Suited for all threaded tips, such as dental probes, PA-probes, brush holders, mirrors, etc. Desinfectable and sterilizable by using any standard procedure.



Handle colors of HELMUT ZEPF GOOL Universal Handles:



See page **03-02** and **03-03** for the article numbers of all **DOM** Handles available.



26.193.20 **SOUR Handle, QUICKEIX, single-ended with end cap**






02-04 Diagnostic

acts according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0

Mouth Mirrors

Due to the standardized thread dimensions, all mirrors available from **HELMUT ZEPF** are compatible with any handle supplied by **HELMUT ZEPF** and can of course be desinfected and sterilized by all usual methods. For fitting handles, please refer to pages **02-03**, **02-05** and for the fitting **ZEPF** 000 H Handle, please refer to page **03-03**.

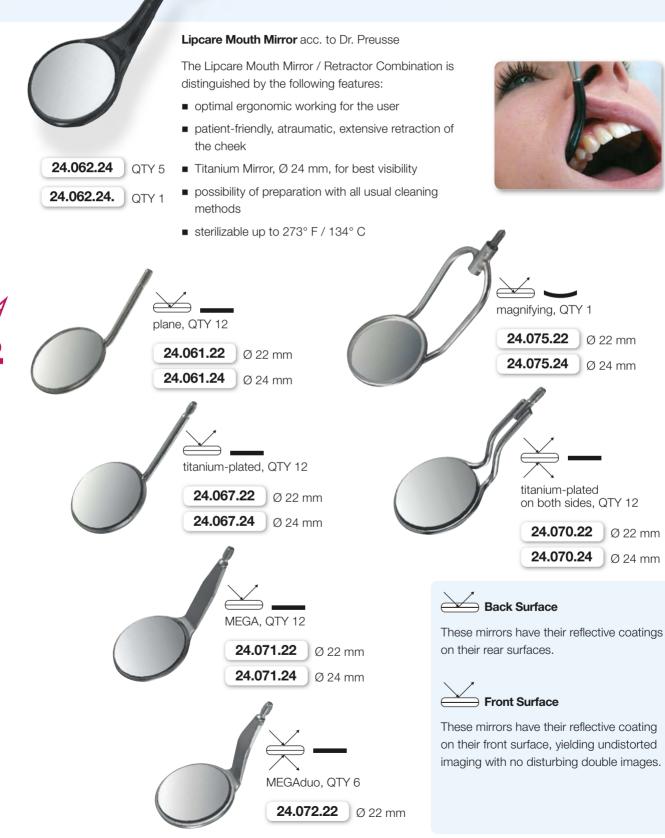

zepf-dental.com

Handle colors of the **HELMUT ZEPF** All-purpose Handles:



Light, manufactured from top-quality plastic with a satin surface finish, ergonomically designed, flexible, suitable for ultrasonic cleaning, sterilizable, and compatible with any standard insert with an M2.5 metric thread.



Retractor acc. to Hilger


This retractor's ergonomically curved surface allows retracting cheeks and tongue under all kinds of working conditions and is also very comfortable for patients, thanks to its convex rear surface and rounded edges.

Interchangeable Probe Tips

Probe Tips, interchangeable. Compatible with any standard handle with an M2.5 metric thread.

The two **ZEPF** Safety Keys to exchange tool ends are illustrated on page **03-05**.

For fitting handles, please refer to pages **02-03**, **02-05** and for the **ZEPF OOK** Handle, please refer to page **03-03**.

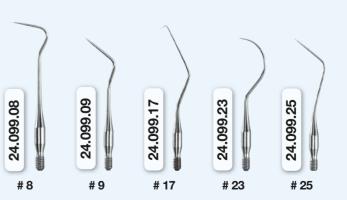

Diagnostic 02-05

26. 191.04

26.191.02

-26: 191.01

26.191.03

⁰²⁻⁰⁶ Diagnostic

+49 (0) 74 64 / 98 88 0

ZEPF Retractor and Mouth Mirror by Dentist Beck

The **ZEPF DONK** Retractor and Mouth Mirror is available in two sizes, featuring a heart-shaped, ergonomic and highly polished design.

The instrument is available in size 24 and 27 mm.

It is universally applicable as:

- Mouth mirror, cheek or tongue retractor, mucoperiosteal flap retractor.
- Its innovative heart shape allows ergonomic adaption in all quadrants.
- Due to its reflective surface, the retractor allows an optimal illumination of the surgical site.
- The large contact surfaces make the retractor very patient-friendly.





CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

ZEPF Photography and Cheek Retractor,

Diagnostic 02-07

in the Onyx Version or stainless steel

HELMUT ZEPF Cheek Retractors are frequently used in intraoral photography, in extensive cheek retraction, in dental diagnostics and in surgery.

Conventional retractors are also available in plastic material. However, depending on the used plastic, these are not always entirely harmless when being prepared in the hygiene chain. Our retractors are made of stainless medical steel and fulfill all the requirements of the RKI guidelines.

The ergonomic design of the retractors guarantees an optimal handling and is well accepted by patients.





All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰²⁻⁰⁸ Diagnostic

+49 (0) 74 64 / 98 88 0

ZEPF Dental Tweezers

All HELMUT ZEPF Dental Tweezers have guide pins that prevent their tips from crossing.

The broader version with its shorter tips allow an application with more pressure compared to common tweezers.









zepf-dental.com

Diagnostic 02-09


ZEPF Ergonomic Dental Tweezers

Our extra comfortable **HELMUT ZEPF** Ergonomic Dental Tweezers are pleasant to hold and have been specially designed for use in extended, otherwise tiring, applications.

The broader version with its shorter tips allow an application with more pressure compared to common tweezers.








ZEPF Medical Probes

Those HELMUT ZEPF Probes shown in figures 8, 9, 17 and 23 are available in octagonal and cylindrical versions, both of which are pleasantly lightweight. Our ergonomically designed octagonal handles are comfortable to hold, and provide precision fingertip control.

Their thin, unbreakable, yet flexible tips manufactured from special alloy steel have an extremely long service life.





K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Periodontology 03-01

ZEPF Periodontal Probes

The perio-diagnostics should be done regularly to have a permanent record to make sure that gingival and especially periodontal inflammations are diagnosed at an early stage.

The benefit for the patient is that either the periodontal health can be confirmed or infection is detected early. Like that suitable dental treatments can be initiated to cure the infection or to stop the progression. With the new Contrast PA Probe Inserts an even easier visualisation is guaranteed during the examination.

The graduation (3 mm) of the probe is visible at the deepest point of the sulcus of all measuring points. Calculus or defective restoration margins cannot be detected, the gingiva is healthy, no bleeding after (careful) probing = no treatment necessary, further preventive care.

Deeper measurements (> 3 mm) indicate a gingivitis. According to the depth further evaluation and documentation must take place according to the rules of the PSI.

See page **03-08** for article numbers of the different **ZEPF** Contrast Probes.



U

H.ZEPF 24,45102

reddot design award winner 2010 All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰³⁻⁰² Periodontology

+49 (0) 74 64 / 98 88 0

reddot design award winner 2010

blonk Universal Handle made of PEEK high-tech plastic material – guarantees an ideal power transmission with formerly unknown sensitivity. The handle is available in 10 different, fresh basic colors.

- Internal	MINISPINIST	- Maria	1
	Manager and South	2 1184	:
-1211	- North Street	2 100	I
	ST ALBORT	100	:
and shall	and the second second	2 110	
	The second second	200	t
a serve	No. of Concession, Name	2711	•
	PERSONAL PROPERTY AND	2,00	2
2011	IN HERPS		9
a fotolide	Contraction of the	2 73 m	I

yellow signal orange red-purple signal purple lightred-magenta turquoise-brightblue cobalt-blue yellow green grey black

	versal Handle
QUICK FIX ,	double-ended

26.193.01
26.193.02
26.193.03
26.193.04
26.193.05
26.193.06
26.193.07
26.193.08
26.193.09
26.193.10

QUICKFIX

All QUICK **FIX** Handles have a metric thread M4 x 0.5 and are therefore compatible with the most common exchangeable inserts.



DODE ID Plug for an individual color coding of the handle series. Material: PEEK high-tech plastic.

Optional, the handle is available with a different colored ID Plug. When placing an order of blonk Handles please indicate the desired **ID-Plug** separately according to the listing below.

	26.195.01
	26.195.02
	26.195.03
	26.195.04
	26.195.05
	26.195.06
	26.195.07
	26.195.08
	26.195.09
6	26.195.10

CC All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

Periodontology 03-03



Universal Handle single-ended QUICKFIX for all common curette and scaler tips including 1 end cap

	26.193.11
(26.193.12
(26.193.13
(26.193.14
(26.193.15
ĺ	26.193.16
	26.193.17
(26.193.18
(26.193.19
	26.193.20


Universal Handle single-ended for exchangeable inserts M2.5, for all common probes and mouth mirrors including 1 end cap and 1 reduction insert 26,194,01

	20.134.01	J
	26.194.02)
(26.194.03)
ĺ	26.194.04)
ĺ	26.194.05)
ĺ	26.194.06)
ĺ	26.194.07)
(26.194.08)
(26.194.09)
ĺ	26.194.10)



Reduction Insert to reduce thread from M4 x 0.5 to M2.5. which enables the use of a double-ended handle for probes and mouth mirrors.

Universal Handle double-ended for exchangeable tips, M2.5, incl. 2 reduction inserts




└───────────── (Length 25 mm) for using the handles as single-ended handle variants.



⁰³⁻⁰⁴ Periodontology

+49 (0) 74 64 / 98 88 0

Comparison of the handles with exchangeable working tips M4 x 0.5 mm

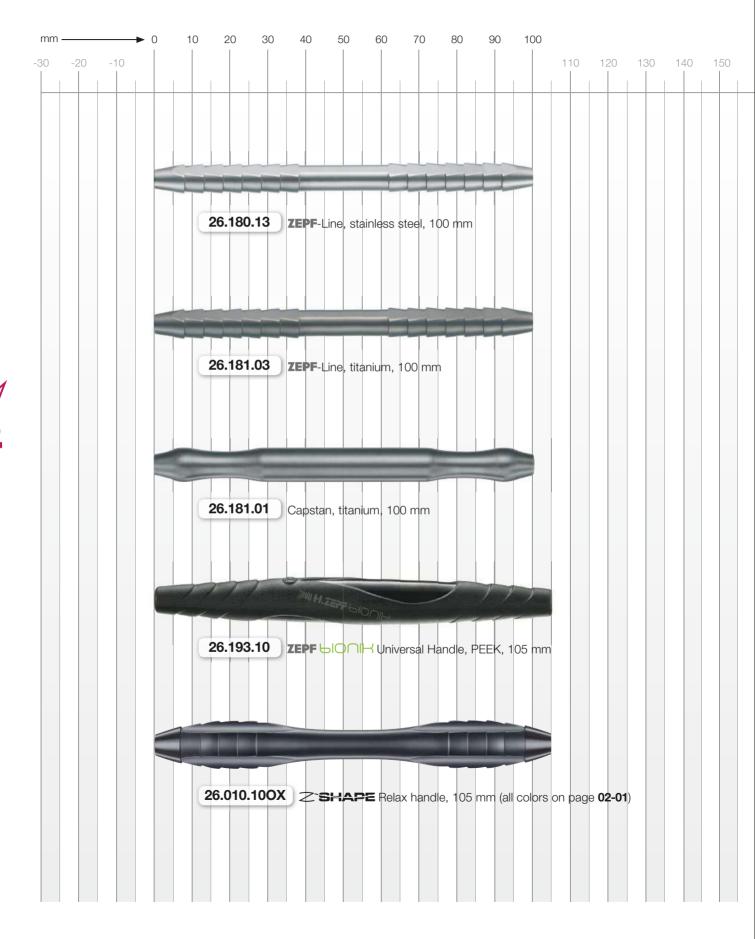

Safety Key with wings to exchange tool ends

24.755.02

Safety Key to exchange tool ends

24.755.03

1

zepf-dental.com

Periodontology 03-05

ZEPF Safety Keys with and without side wings

The Safety Key holds the tips firmly in place. The side wings (only **24.755.02**) protect from potential injuries due to the extremly sharp cutting edges of the tips.

Exchanging of Inserts



Start by screwing the tip (sharp end) carefully by hand into the handle. Make sure that only the handle is turned. Not the tip.





Pull in the tip with the **ZEPF** Safety Key. With the other end, proceed as before. To set the tips, it is better to use two Safety Keys.



The Safety Key holds the tips firmly in place. The side wings protect from potential injuries due to the extremly sharp cutting edges of the tips.

⁰³⁻⁰⁶ Periodontology

+49 (0) 74 64 / 98 88 0

Gracey M5 Prophylaxis Set in Z^{SHAPE} or **GOOK** handle with **ZEPF** nangpau^e coating

Small Instrument Set optimally compiled for Deep Scaling, consisting of M5 Gracey Curettes figures 1/2, 7/8, 11/12, 13/14 and a Sickle Scaler # 204S for application in all quadrants.



K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Periodontology 03-07

Alternative Instruments:

in \geq SHAPE or **GOOK** handle with **ZEPF** nangpause coating

For the Gracey M5 Prophylaxis Set. Sickle Scaler # 204 SD and Sickle Curette (Molar Scaler) # M 23A





24.989.55OX


ZEPF Prophylaxis Set 'M5 Deep Scaling' in **∠**⁻**SHAPE** RELAX handle, complete with nanopau[®] coating

24.990.55OX

 ZEPF Prophylaxis Set 'M5 Deep Scaling'

 in ZEPF 6001K handle, inserts

 with nanopau* coating



HELMUT ZEPF M5 Curettes have a 1st shaft which is about 3 mm longer. The sharpened instrument tip is shortened as to allow a special subgingival curettage for tight and deep pockets as well as narrow root surfaces. All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E (ϵ) are mentioned in the index from page 11-07.

⁰³⁻⁰⁸ Periodontology



Contrast PA Probe Inserts

The new **ZEPF** Contrast PA Probes are made of plastic material and have a flexible working tip which adapts optimally to the anatomy of the pocket depth when measuring.

Colorstable, black markings on the white basic material guarantee a very good contrast for reading.

The sterilizable, exchangeable tips are available in different common graduations.


They are suited to determine the parodontal status and especially to be used on implants. Scratching of implant surfaces is avoided with these probes.

The tips are reusable until they bend, the color fades or the graduation is not readable any more.









graduation 3/6/8/11 mm M4 x 0.5 mm, PU 12 pieces



graduation 3/6/9/12 mm M4 x 0.5 mm, PU 12 pieces






graduation 2/4/6/8/10/12 mm M4 x 0.5 mm, PU 12 pieces









M4 x 0.5 mm, PU 12 pieces





graduation 1 - 15 in mm steps, North Carolina M4 x 0.5 mm, PU 12 pieces









⁰³⁻¹⁰ Periodontology

) E

+49 (0) 74 64 / 98 88 0

Periodontal Probes

All **HELMUT ZEPF** Periodontal Probes are high-speed machined. Their tips are thus very fine and dimensionally accurate to within very high tolerances. All our PA-Probes have markings that are suitable for ultrasonic cleaning. Our WHO Periodontal Probes have spherical tips.

They are particularly ideal for:

- determining papillary
- bleeding indices, and their "stops" (the balls on their tips) prevent injuries when measuring the depths of pockets, i.e., they are more atraumatic than other types of PA Probes.

24.453.03 CP 11.5 (WHO) graduation 3.5/5.5/8.5/11.5 mm 24.453.12 CPG 12 graduation 3/6/9/12 mm 24.453.22 CPN 22 graduation 2/4/6/8/10/12 mm 24.453.23 University North Carolina, CNC graduation 1 - 15 mm, in mm steps

zepf-dental.com

Periodontology 03-11

Periodontal Screening Index, PSI

For using the periodontal screening index, it is necessary to use the WHO probe. The steel ball at the distal end of the probe features a diameter of 0.5 mm.

The steel ball avoids not only injuries but allows to discover rough surfaces and edges of dental fillings. The first measurement area of the probe is a black 2 mm band, which shows the depth from 3.5 mm up to 5.5 mm. For further information, please check the relevant description of the periodontal screening index (PSI).

24.454.01 CPG 12

graduation 3/6/9/12 mm The **ZEPF** IONIK Handle is available in 10 different colors. See page **03-02** and **03-03** for the article numbers of all IONIK Handles available.



24.454.02 CPNG 22

graduation 2/4/6/8/10/12 mm








graduation 3.5/5.5/8.5/11.5 mm



24.454.05 Williams graduation 1/2/3/5/7/8/9/10 mm





graduation 1 - 15 in mm steps, North Carolina



24.454.06TI CNC

graduation 1 - 15 in mm steps, North Carolina, titanium

All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E (ϵ) are mentioned in the index from page 11-07.


⁰³⁻¹² Periodontology



K2019-03/1-E CC All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Periodontology 03-13

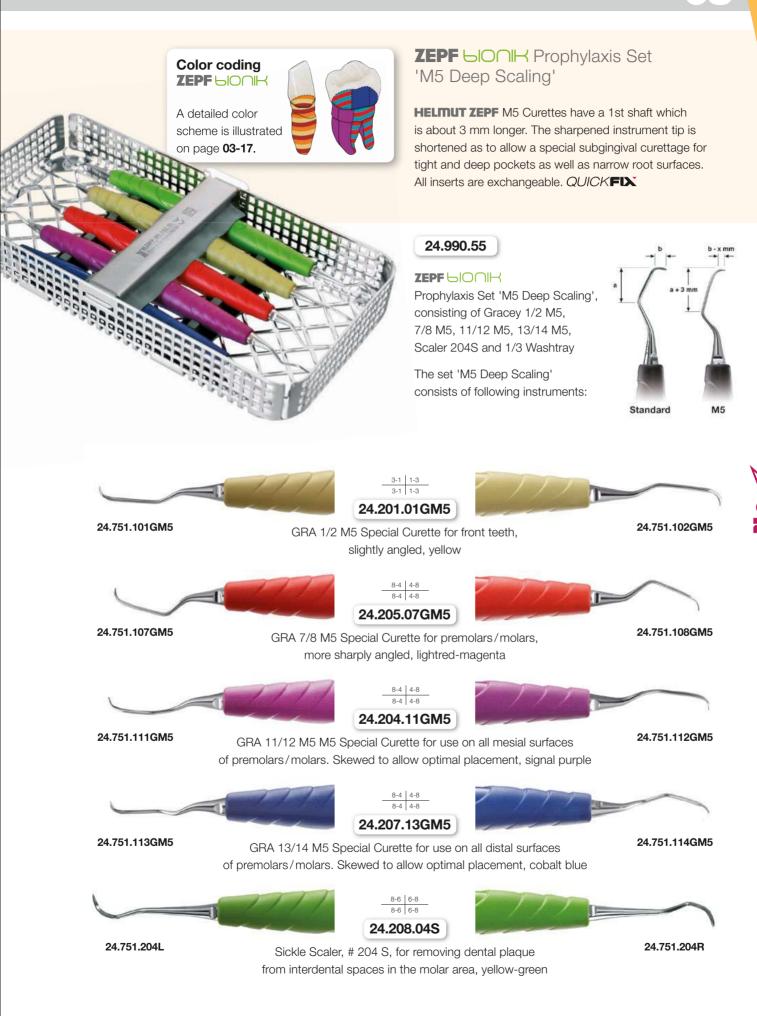

All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E $C \in$ are mentioned in the index from page 11-07.

⁰³⁻¹⁴ Periodontology



ZEPF GOOK Prophylaxis Set

Unlike Gracey Curettes, HELMUT ZEPF Universal Curettes have two working surfaces or cutting edges. The Universal Set allows a quick and efficient prophylaxis

consisting of Langer 1/2, 3/4, 5/6, M23, Universal Curette 204S and 1/3 Washtray.

consists of the following instruments:



24.751.123L

24.751.204L

24.207.23



M 23 Universal Curette for use on upper and lower side teeth and supragingival dental plaque. Slim version, cobalt blue

24.751.123R



Sickle Scaler, # 204 S, for removing dental plaque from interdental spaces in the molar area, yellow-green

24.751.204R

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Periodontology 03-15



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰³⁻¹⁶ Periodontology

+49(0)7464/98880



winner 2010

reddot design award

ZEPF 600 Gracey Special Curettes

HELMUT ZEPF Gracey Curettes are special Curettes that have just a single working surface or cutting edge, and are thus suitable for removing concrementations or dental plaque only.

The **ZEPF** Handles are available in 10 different colors.

See page **03-02** and **03-03** for article numbers of the different color and handle versions. *QUICK***FIX**



K2019-03/1-E C All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Color Coding **ZEPF** 600 Gracey Special Curettes



All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E CE

⁰³⁻¹⁸ Periodontology

McCall, # MC 13S/14S, Scaler for use on interdental spaces

on front teeth and premolars, cobalt blue



winner 2010


reddot design award

ZEPF GOOK Universal Curettes

Unlike Gracey Curettes, HELMUT ZEPF Universal Curettes have two working surfaces or cutting edges, and thus allow using the same instrument on mesial and distal surfaces. All inserts are exchangeable.

The **ZEPF** | O | Handles are available in 10 different colors.

See page 03-02 and 03-03 for the article numbers of all **DONK** Handles available. QUICKFIN

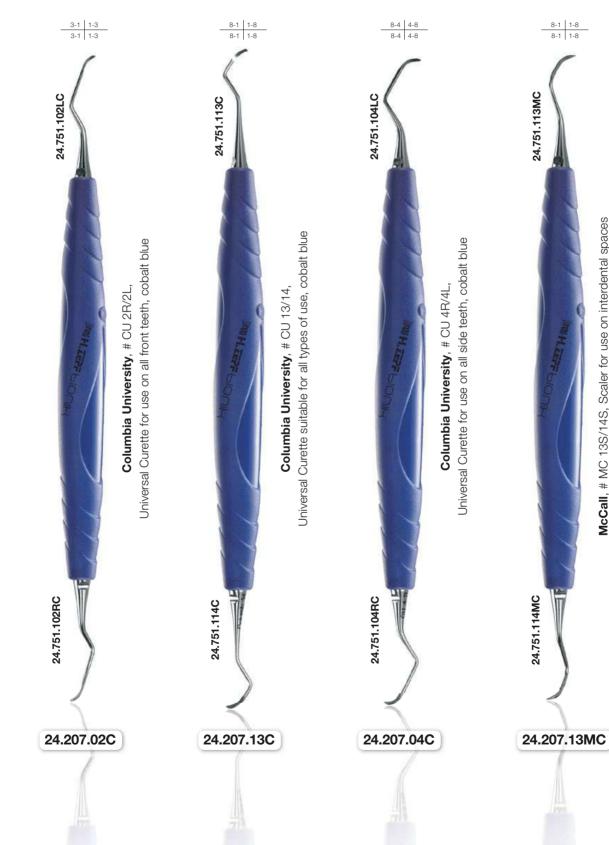

All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E CE

Periodontology 03-19



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰³⁻²⁰ Periodontology

+49 (0) 74 64 / 98 88 0



winner 2010

reddot design award

ZEPF GOOR Universal Titanium Curettes \vec{D}

Universal Curettes with exchangeable, very delicate titanium inserts from **HELMUT ZEPF**, to remove the accumulated plaque film on the implant necks. The titanium inserts are exchangeable.

The **ZEPF** Handles are available in 10 different colors. See page **03-02** and **03-03** for article numbers of the different color and handle versions. *QUICK* **FIX**



Periodontology 03-21



ZEPF 600 MS Titanium Curettes 7

HELMUT ZEPF M5 Curettes have a 1st shaft which is about 3 mm longer. To remove the accumulated plaque film on the implant necks. The titanium inserts are exchangeable. The **ZEPF** ||O ||| Handles are available in 10 different colors.

See page 03-02 and 03-03 for article numbers of the different color and handle versions. QUICKFIX





F

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰³⁻²² Periodontology

+49 (0) 74 64 / 98 88 0



ZEPF 600K Scaler

red<mark>dot</mark> design award winner 2010 **HELMUT ZEPF** Sickle Scalers have ultrafine tips for supragingival use. Unlike Jacquette scalers, they have curved facial surfaces. With blunt tips, for general use.

All inserts are exchangeable.

The **ZEPF bloold** Handles are available in 10 different colors.


See page 03-02 and 03-03 for article numbers of the different color and handle versions. QUICKFIX










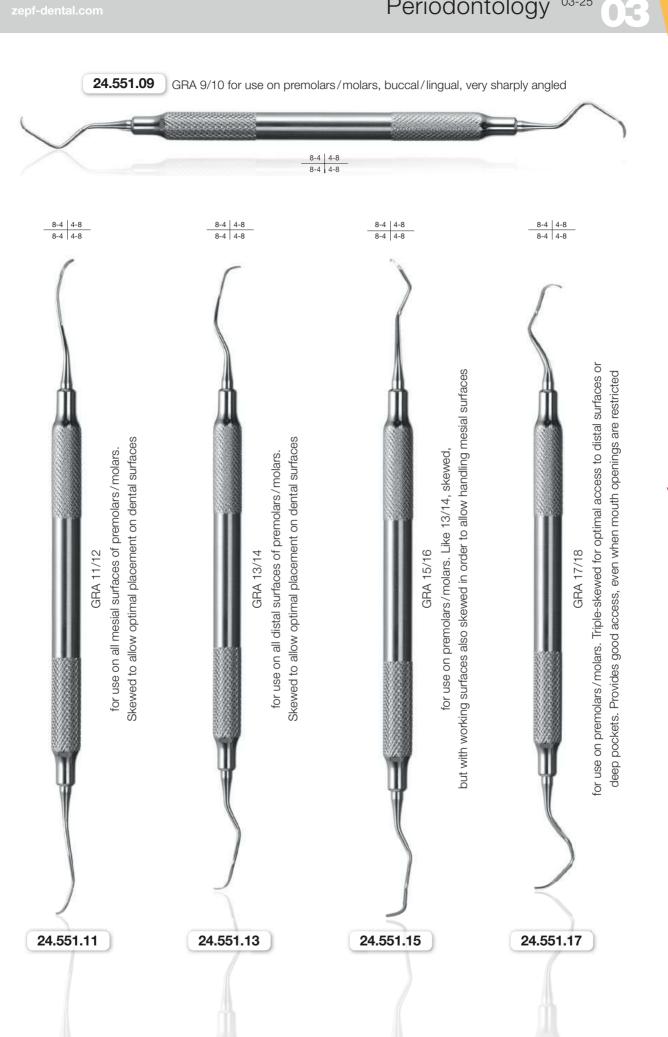

Periodontology 03-25





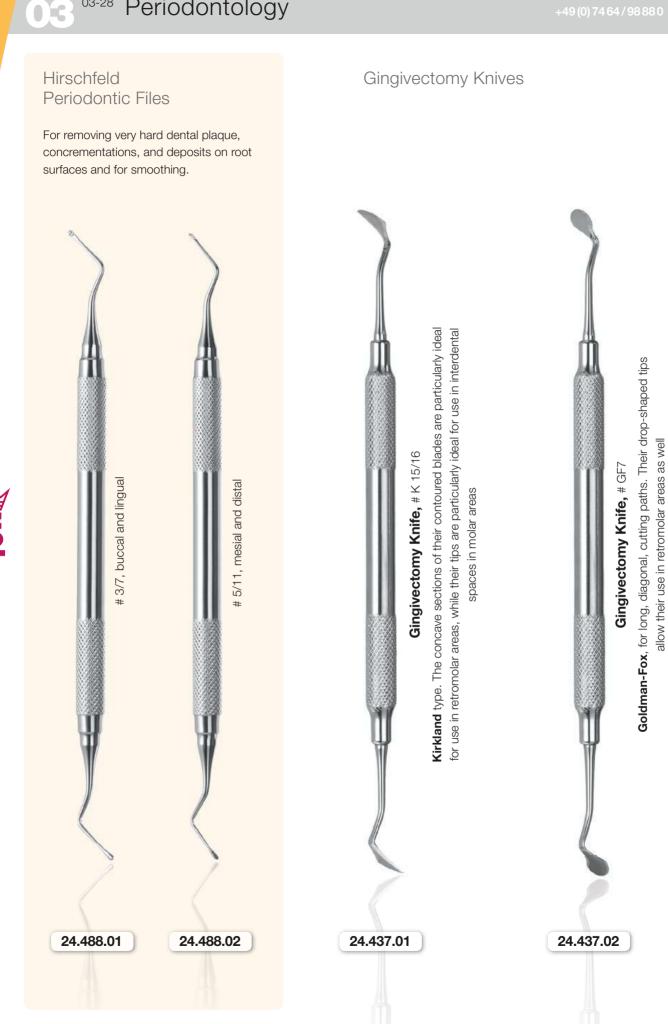

All CE marked products according to the Medical Device Directive 93/42/EEC ce are mentioned in the index from page 11-07.

⁰³⁻²⁸ Periodontology

K2019-03/1-E



⁰³⁻³⁰ Periodontology

+49 (0) 74 64 / 98 88 0

Periodontal Chisels






zepf-dental.com

Periodontology 03-31

I

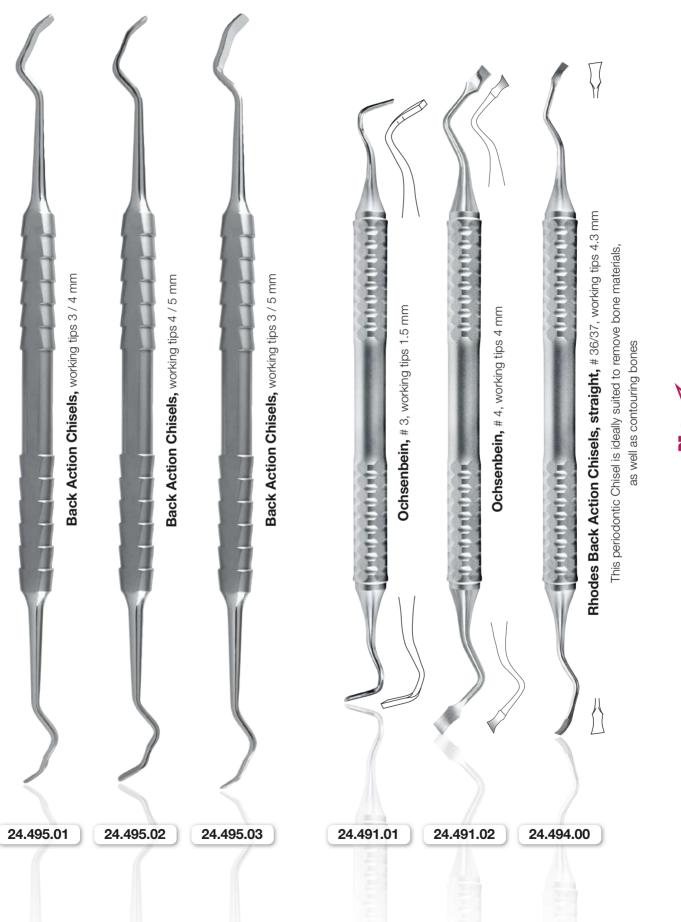

⁰³⁻³² Periodontology

Original Arkansas Sharpening Stones





24.926.75

Test Probe, Acryl Glass 76 x 6 mm, PU = 6 pieces



24.950.00

Sharpening Oil 100 ml, for Original **ZEPF** and Arkansas Stones

24.951.01

with screw.

Vise



zepf-dental.com

Periodontology 03-33



Original Arkansas Stone

The diameter of the Original Arkansas Stone is designed to fit the contour of the working ends of our luxation elevator 17.006.01 to 04 and those of our **ZEPF** Xtool-Elevator 17.007.01 to 07.

So do sharpen your luxation elevators regularly! The best results can be obtained in combination with our Sharpening Oil 24.950.00.




ZEPF Sharpening Stones

Just sharp instruments! Oxide ceramic sharpening stone with extraordinary hardness. Highest resistance to wear and tear and to deformation, to achieve an excellent surface quality when grinding. The low wear properties provide attractive economic advantages in comparison to customary Arkansas sharpening stones.



All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E are mentioned in the index from page 11-07.

⁰³⁻³⁴ Endodontics

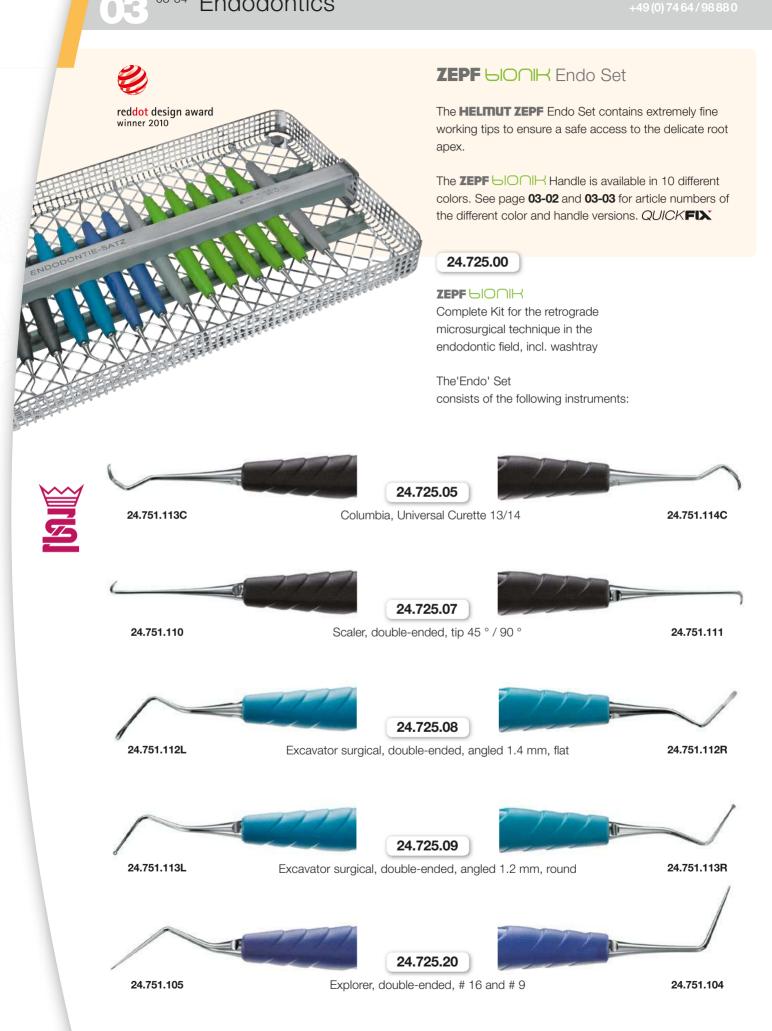



⁰³⁻³⁶ Endodontics

+49 (0) 74 64 / 98 88 0

Anatomical Plate Forceps for all Endo purposes

Anatomical Plate Forceps acc. to Dr. Dirk Brozio

The full area contact generated by compressing the tweezers, ensures a safe support in each gripping angle. The Plate Forceps are featuring a much higher safety when gripping, holding and positioning fine and delicate objects. This problem has been solved by the patented design of the Plate Forceps as their working tips have circular surfaces with additional serrations inside. Easy and relaxed handling due to low holding forces to allow a safe and fast treatment.




留H.ZEPF 122.107.21 ℃ 整 Mote in Germany 13017 ℃ 22.107.21 Anatomic Plate Forceps 180 mm





19.649.60


Surgical Aspirator

with Luer Connector, curved, optimal for Endo-Tips, 175 mm long, Ø 4.2 mm

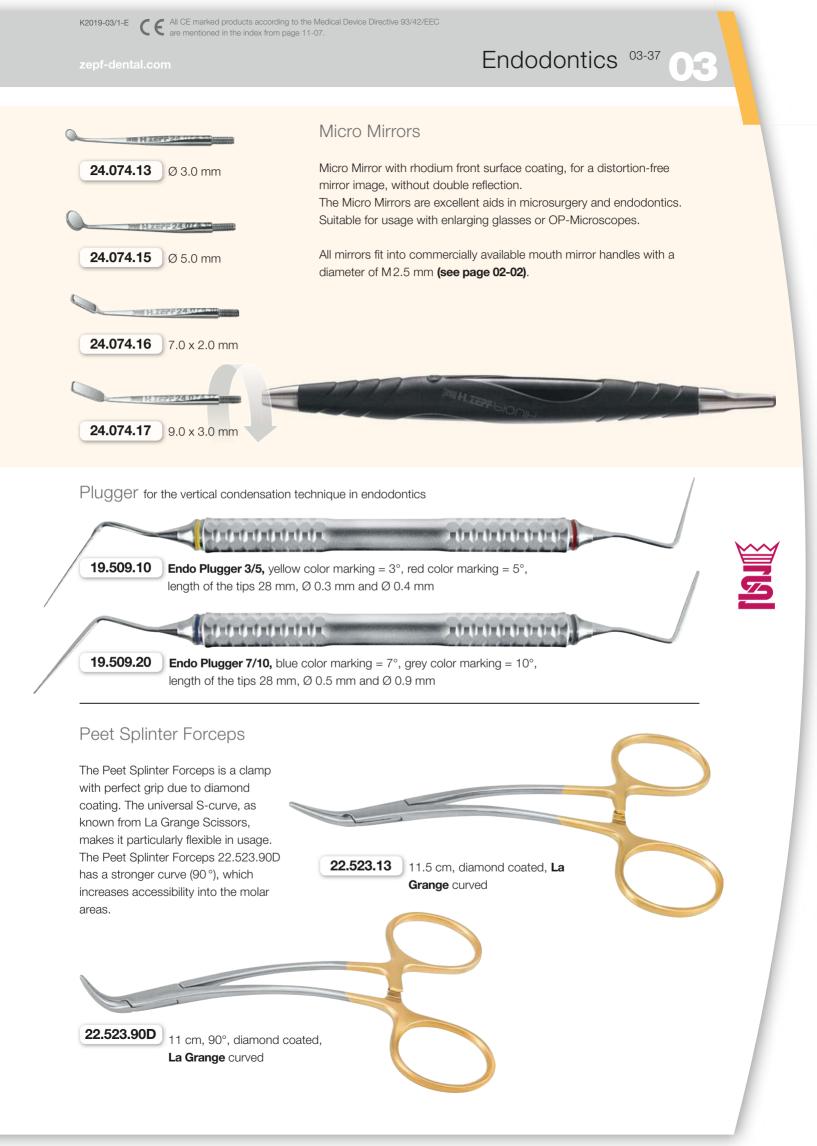

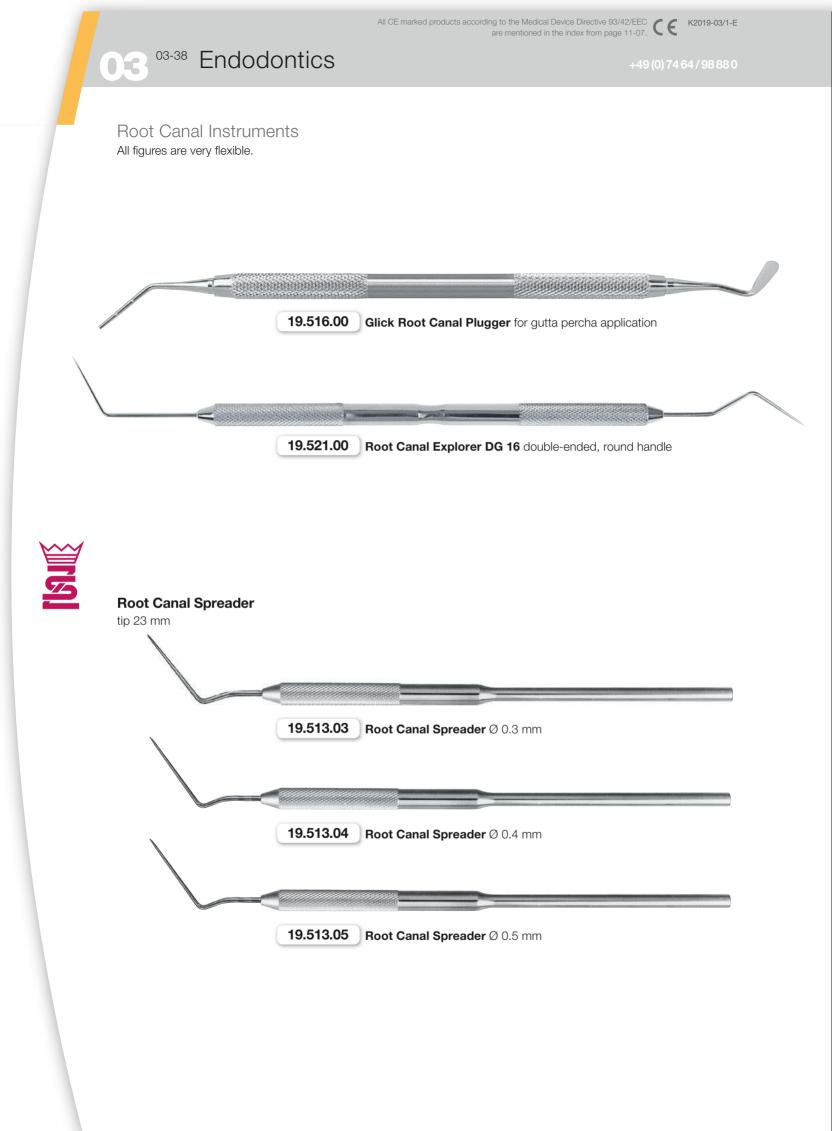

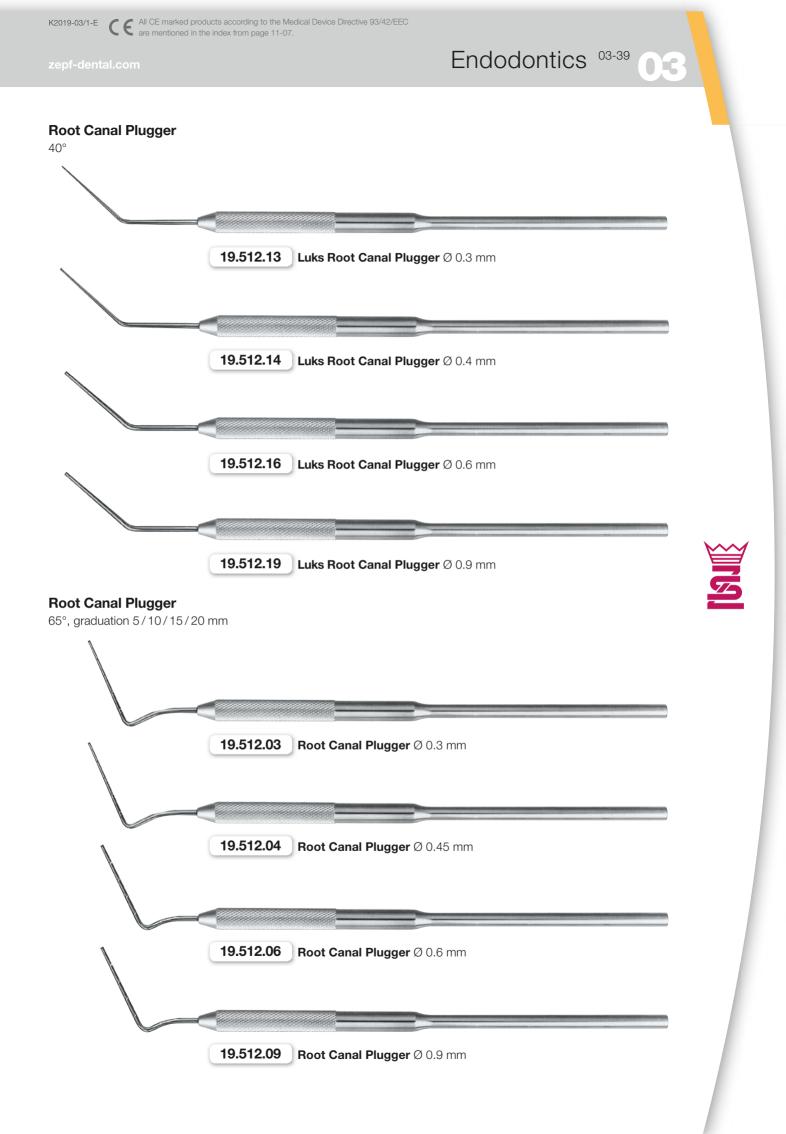

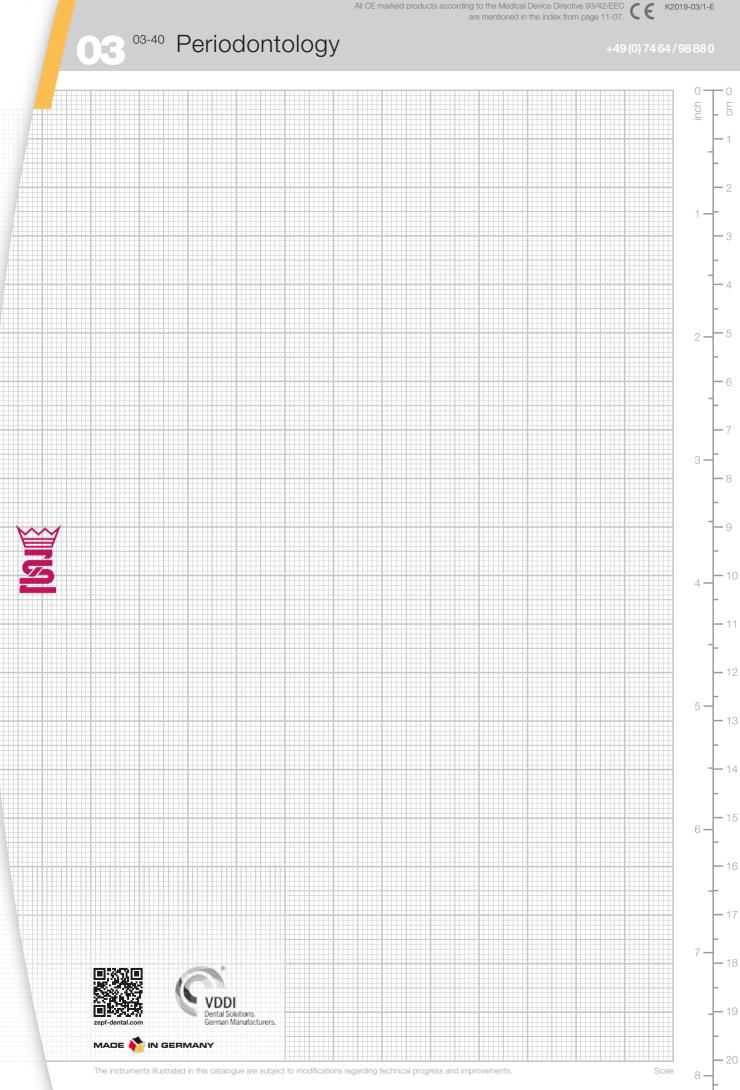

zepf-dental.com

Conservation 04-01

ZEPF **GOOK** Composite Sets

All Composite Tips feature the special **ZEPF** Onyx coating. The reflection-free **ZEPF** Onyx coating is extra smooth, harder and more scratch-resistant than conventionally coated composite instruments. The popular handles in the **ZEPF DONK** design are made of lightweight, highquality plastic material.

The **ZEPF 6 O 1H** Handles are available in 10 different colors. See page **03-02** and **03-03** for article numbers of the different color and handle versions.



reddot design award winner 2010

19.202.00

CompoSMOOTH Complete Set

by Prof. Dr. Gabriel Krastl incl. Washtray 1/3 and Soft Application Inserts in a box, as described on pages **04-02** to **04-05**

26.120.01Ti

Small Composite Set incl. Washtray 1/3 as described on pages 04-02 to 04-05



26.120.00Ti

-

Big Composite Set incl. Washtray 1/2 as described on pages **04-02** to **04-05** 04-02 Conservation

All CE marked products according to the Medical Device Directive 93/42/EEC $\,$ CE $\,$ K2019-03/1-E $\,$ are mentioned in the index from page 11-07. $\,$

+49 (0) 74 64 / 98 88 0

The ZEPF SIONIC Composite Sets

26.120.01Ti	Small Composite Set
26.120.00Ti	Big Composite Set
19.202.00	CompoSMOOTH Set

The sets contain the accordingly marked Composite Instruments **X X** :






CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

04-04 Conservation

+49(0)7464/98880

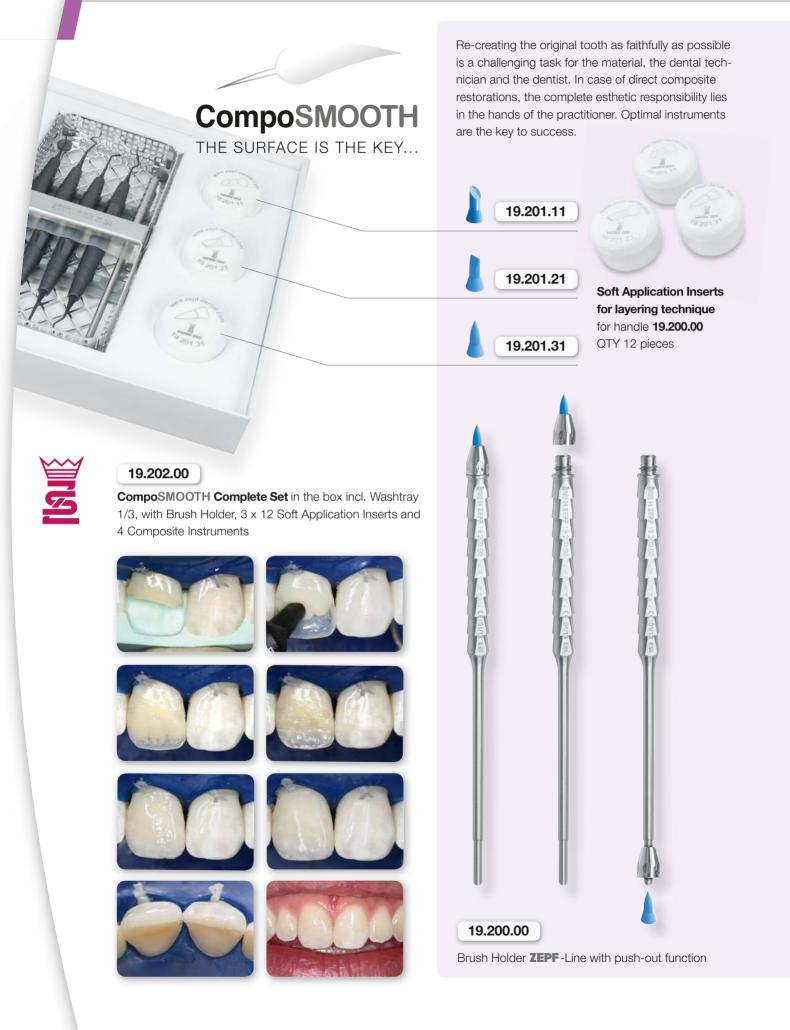

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Conservation 04-05

The new **CompoSMOOTH**, a special silicone brush, allows an effortless adaptation and modelling of the composite surface before polymerization. Even "sticky" composites can be adapted in an optimal way. The perfect surface morphology is created almost automatically by light pressure. The tooth shape is modeled in a way that reduces the subsequent polishing work to a minimum... and the result – optimal!





Brush Holder 30° Optionally available

HELMUT ZEPF developed

this brush holder which is bent by 30° to get an optimal result in difficultto-reach places. This instrument is not included in the set, but it can optionally complete the set in a profitable way.

19.200.30

Brush Holder curved 30° **ZEPF**-Line with push-out function

ATTIN Compo Knife for mesial and distal surfaces, in ZEPF UOMH Handle yellow greer

exchangeable inserts with nanapaus coating

24.710.02OX

ATTIN Compo Knife for buccal and lingual surfaces, in ZEPF SIONIN Handle black,

24.710.01OX

exchangeable inserts with nanapau" coating

04-06 Conservation

+49 (0) 74 64 / 98 88 0

ATTIN Compo Knives to remove composite residues in filling treatment

With the ATTIN Compo Knives in the **ZEPF GONK** Handle, instruments have been specially developed for removing composite filling residues. Coated with **Danapa** these instruments have a surface hardness of 4500 Vickers. Every dentist removes composite filling residues in different ways. Some use curettes, others excavators and sometimes scalpel blades are used. Curettes and scalers are usually too weak, i.e. there is a high risk of breakage. Scalpel blades have a high level of hardness, are correspondingly sharp and are good to use. But there are only a few angles available, so they do not allow ergonomic working.



The new ATTIN Compo Knives have addressed this requirement, i.e. strong blades manufactured at the correct angles, so all quadrants can be optimally reached.

With the new **ZEPF** coating, the surface has a hitherto unknown hardness.

The cutting performance is therefore guaranteed for a long period. Should an insert ever become blunt, it is easy to replace only this instrument insert.

Advantages:

- Only two instruments for all quadrants
- ZEPF Cance and lifetime
- Instrument inserts are exchangeable
- Non-light reflecting surface



reddot design award

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Micro-composite Spatulas –

superfine spatulas with **ZEPF**



In the case of direct composite restorations, the entire aesthetic responsibility lies in the hands of the practitioner.

With the new micro-composite spatulas in 1.1 mm and 1.6 mm, the practitioner is provided with highly flexible ultra-fine spatulas for precise modeling of delicate structures.



The new **ZEPF** nanapat[®] coating offers you a very good contrast to the used material. The polished surface is easy to clean and extremely scratch resistant.



block Universal Handle made of PEEK high-tech plastic material – guarantees an ideal power transmission with formerly unknown sensitivity. The handle is available in 10 different, fresh basic colors.

The exchangeable working tips inserted in the ergonomic **DONK** handle offer highest economy and best tactile handling.



Conservation 04-07





04-10 Conservation

+49 (0) 74 64 / 98 88 0

Spatula

13

26.200.13

fine version, 1.6 mm

02

Condenser

HELMUT ZEPF Filling Instruments are well-balanced, i.e., the offsets of their blades are symmetric about the longitudinal axes of their handle, which keeps their blades from twisting under load.







⁰⁴⁻¹² Conservation

+49(0)7464/98880

Excavators

04

Excavators in different angles to remove softened dentine during cavity preparation.





Conservation 04-13

4

04-14 Conservation

а

Anatomic Ehricke for Upper Jaw

The choice of the impression tray and the impression technique will influence the final result significantly. If polyethers are used, we are recommending non-perforated impression trays.

28.631.01

28.631.04

28.634.02

a = 68 mm,

b = 61 mm,

SUP U2

a = 65 mm,

b = 52 mm,

a = 80 mm,

b = 73 mm,

SUP B4

SUP B1

Regulars (BO)





F



D				
Partials,	depressed	centers	(PO)	



28.632.01
a = 62 mm,
b = 51 mm,
SUP P1

28.631.00

28.631.03

28.63
a = 72 r
b = 54 r
SUP P2

32.02 mm, mm,

28.632.03 a = 73 mm, b = 60 mm,SUP P3

28.631.02

28.634.03

a = 72 mm,

b = 65 mm,

SUP U3

a = 71 mm,b = 60 mm,

SUP B2

28.633.03
a = 77 mm,
b = 63 mm,
SUP F3



Functional impressions (FO)

28.633.01				
a = 61 mm,				
b = 50 mm,				

SUP F1


a = 67 mm, b = 55 mm, SUP F2

28.633.02



zepf-dental.com

Conservation 04-15



Regulars (BU)



Edentulous (UU)



Anatomic Ehricke for Lower Jaw

The choice of the impression tray and the impression technique will influence the final result significantly. If polyethers are used, we are recommending non-perforated

impression trays.

28.636.00

28.636.03

28.638.01

a = 71 mm.

b = 58 mm,

INFU1

a = 61 mm,

b = 44 mm,

a = 82 mm,

b = 58 mm,

INF B3

INF B0

28.636.01 a = 72 mm,

b = 51 mm, INF B1

28.636.04 a = 83 mm,

28.638.02

a = 70 mm.

b = 58 mm,

INF U2

b = 65 mm, INF B4



28.638.03 a = 74 mm, b = 59 mm, INF U3



Partials, depressed centers (PU)



28.637.01 a = 64 mm, b = 53 mm, INF P1

28.637.02 a = 71 mm.

a = 71 mm, b = 59 mm, INF P2

28.637.03


a = 80 mm, b = 59 mm, INF P3

Modeling Knife for Impressions

Silicone Knife with cutting loop.

28.121.00

04-16 Conservation



Perforated Anatomic Ehricke for Upper Jaw

A-Silicone putties can be applied in perforated impression trays, as the perforation intensifies the rotation of the material in the impression tray.

Regulars	(BO)
----------	------



Edentulous (UO)

a = 65 mm, $b = 56 \, \text{mm},$ SUP U1

28.604.01

28.601.00

28.601.03

a = 65 mm,b = 52 mm, SUP B1 28.601.04

28.601.01

a = 80 mm, b = 73 mm, SUP B4

28.604.02

a = 68 mm,

b = 61 mm,

SUP U2

28.601.02

a = 71 mm,b = 60 mm,SUP B2

	2	8.6	04.03
а	=	72	mm,
b	=	65	mm,

SUP U3



Partials, depressed centers (PO)





28.602.03

a = 73 mm, b = 60 mm,SUP P3

Functional	impressions	(FO)
------------	-------------	------



	28.6	603.01	
а	= 61	mm,	

b = 50 mm, SUP F1

C	28.6	03.02
а	= 67	mm,

b = 55 mm, SUP F2

28.603.03

a = 77 mm, b = 63 mm, SUP F3

Perforated Anatomic Ehricke f

A-Silicone putties can be applied in perforated impression trays, as the

Conservation 04-17

Regulars (BU)



Edentulous (UU)



for Lower Jaw		
A Silicopo puttios con bo applic	d ii	o r

perforation intensifies the rotation of the material in the impression tray.

28.606.00
a = 61 mm,
b = 44 mm,
INF B0

28.606.03

a = 82 mm, b = 58 mm, INF B3

28.608.01 a = 71 mm, b = 58 mm,INFU1

a = 72 mm,
b = 51 mm,
INF B1
28 606 04

28.606.01

28.608.02

a = 70 mm,

b = 58 mm,

INF U2

a = 83 mm, b = 65 mm, INF B4

28.606.02 a = 78 mm,

b = 54 mm, INF B2





Partials, depressed centers (PU)



28.607.01	28.607.02
a = 64 mm,	a = 71 mm,
b = 53 mm,	b = 59 mm,
INFP1	INF P2

28.607.03

a = 80 mm, b = 59 mm,INF P3

04-18 Conservation

Impression Trays for Implantology acc. to Helfgen

■ simple handling

- open and closed implant impression
- putty-wash impression possible
- precision enhancement
- also universally usable in case of special indications
- only one impression session required
- sterilizable
- different sizes
- time and cost efficient



Functionality of the Impression Trays for Implantology acc. to Helfgen



1. In the area of the prepared teeth, retraction cords are placed. Smooth, retention free screws are twisted into the implants.



2. On its lateral sides the covered tray is coated with adhesive. Then the tray is charged with putty material.



3. For the primary impression, the charged tray will be pressed until the cover rests on the smooth implant screws.



4. After the removal of the primary impression, the smooth screws will be exchanged for the complete impression posts.





5. The tray cover is removed and the impressed screw channel is extended with the perforator.




6. For undisturbed repositioning, the perforated channel may be extended further using a super-coarse mill.



7. After the impression areas have been surrounded by ligth-body material, the repositioned impression may be filled additionally via the perforations of the cap channels, if required.



8. Once the material has cured, the positioning screws are loosened, and the finished impression can be removed.

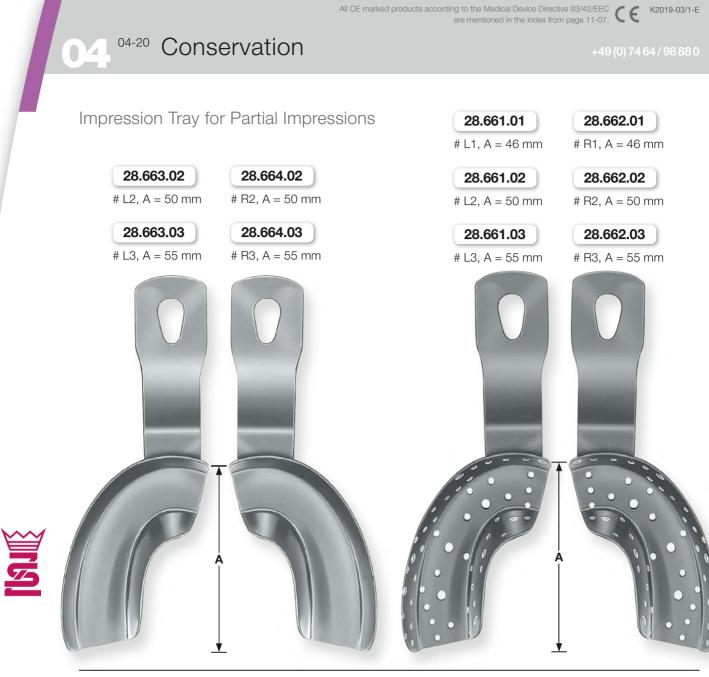

Stolley with screw

28.671.00 perforated

28.672.00 non-perforated



Stolley with bolt

28.681.00 28.682.00 perforated

non-perforated



04-22 Conservation

+49 (0) 74 64 / 98 88 0

MU H. 2007 19,199,00


19.199.00

Brush Holder

Brush Holder **DBGM**

Its most important features...

Our **ZEPF** Brush Holder is used for applying liquid treatment agents (enamel or dentine adhesion agents, acids, lacquers, or fluoridation agents) to dental surfaces or cavities.



2 Back-action-instrument



Its features at a glance

- Includes a dual brush receptacle and an original **ZEPF** scaled handle.
- Universal use on both upper and lower jaws and on all dental surfaces and cavities.
- No need for plastic applicators (reduces waste).
- May be desinfected and sterilized by using any standard procedure.
- Virtually unlimited service life.
- Designed for optimal ergonomy and general-purpose use.
- Suitable for all regular brush inserts (single use).
- Used in all areas of dentistry, especially adhesive restoration work.

К2019-03/1-Е

CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Conservation 04-23

Separation Forceps pat. pend. by Dr. Peter Müller, Ebersbach

Their benefits...

- Innovative, functional design.
- Rapid, safe, efficient spreading.
- Adjustable rest allows supporting them on teeth.
- Good access to interdental spaces during spreading.
- For general-purpose use on upper or lower jaws.
- Substantial time savings.
- Secure, one-handed control.
- For right-handed and left-handed persons.
- Desinfectable and sterilizable by using any standard procedure.



The adjustable rest may also be used to support the teeth at locations remote from the intervention point.

Spread the teeth and insert a matrix into the interdental space.



MESTERN

04-24 Conservation

+49 (0) 74 64 / 98 88 0


Tofflemire Matrix Retainer

Manufactured from stainless steel.



Tofflemire Matrix Bands for 19.060.00

Manufactured from top-quality, 0.035 mm gauge, stainless steel, packaging unit: 12 ea. of each size.

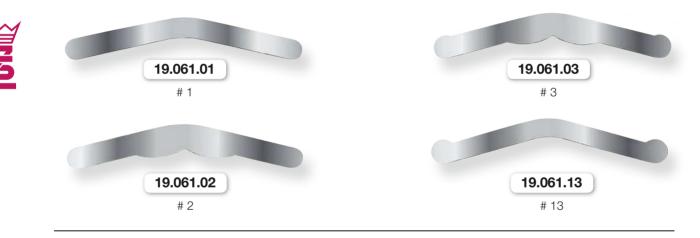

Articulating Paper Forceps



K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Conservation 04-25

EASY CONTACT POINT Instruments by HELMUT ZEPF



Composites are not easy to process. The modeling of clinically ideal contact points in particular is a big challenge for the practitioner. The Easy Contact Point Instruments will help to simplify this work step.
These instruments are available in two sizes as pliers for MOD filling, i.e. as premolar and as molar pliers.
To be used as hand instruments for MO or DO fillings. Also available in two sizes for premolars and molars.
The treatment period for a composite filling can therefore be considerably reduced.
The related economic benefit is evident.

⁰⁴⁻²⁶ Conservation

are mentioned in the index from page 11-07. CC

K2019-03/1-E

+49

All CE marked products according to the Medical Device Directive 93/42/EEC

Universal Finishing Clamp "Work smart not hard"



The **ZEPF** Finishing Clamp is an innovative holding instrument for finishing strips of all kinds. The instrument has been designed with ergonomics and functionality uppermost and contributes significantly to easing work involving finishing strips.

The treatment is pleasant for the patient because the tongue area is not restricted by the dentist's fingers and does not aggravate choking. Its main application is in the area of approximate composite fillings; apart from this the instrument is well suited for separation, the correction of filling surpluses in approximal area as well as the application of dental floss.





ZEPF Finishing Clamp, QTY 2 pieces DBGM by Dr. Peter Müller, Ebersbach



Fields of Application:

- 1) Completion of approximal composite fillings.
- 2) Separating by means of steel-carbon strips or diamond skived steel strips.
- **3)** Correction of filling over-hangs in the approximal area.
- 4) Removal of matrix strips after laying fillings.
- **5)** Clamping dental floss for interdental plaque removal, especially in difficult access spots in the lateral tooth area.
- 6) Clamping dental floss for removal of cement residues from the interdental area after cementing crowns / bridges.




No treatment unit should lack these Universal **HELMUT ZEPF** Pliers and Tweezers. They are used for securely grasping provisional plastic items, bridges, nerve instruments, impacted matrices, attaching inlays, setting interdental wedges, etc. Usable on both upper and lower teeth. Their TC-jaws provide a secure grip.



Peet Splinter Forceps



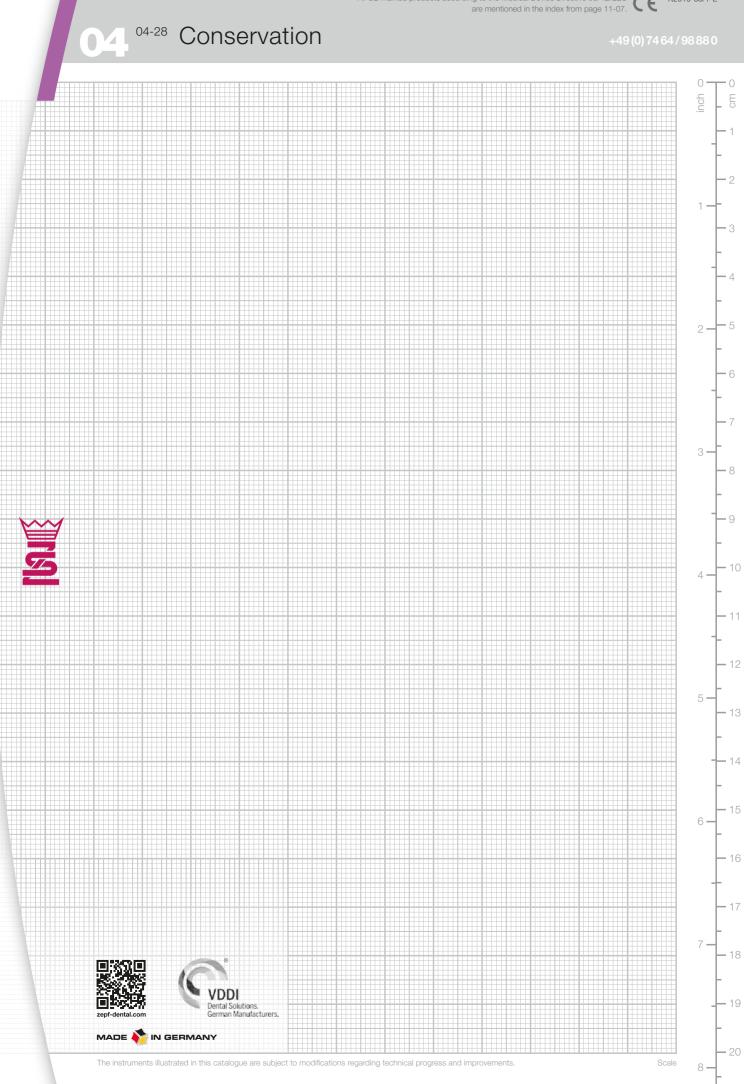

zepf-dental.com

Extraction 05-01

PATENTED

12.300.08

Benex[®]*II* Extractor acc. to Dr. med., med. dent. Benno Syfrig

HZEPF (CE/02/13 12.300.08

Extraction System

acc. to Dr. med., med. dent. Benno Syfrig

Pursuing logically the quest of gentle extraction, **HELMUT ZEPF** Medizintechnik GmbH has developed a new, patented (Pat. No. CH 696 458) **Benex*** extraction system in close collaboration with Benno Syfrig Dr. med., med. dent from Switzerland. You will find further information, application examples and the **Benex*** user forum at:

www.benex-dent.com

05-02 Extraction

K2019-03/1-E



Picture 1 Longitudinal extraction with Benex*II step by step: Pivot tooth extracted due to root fracture



Picture 2 Longitudinal extraction with Benex*II step by step: Axial removal



Picture 3 Longitudinal extraction with Benex II step by step: Soft and hard tissues preserved



Picture 4 Longitudinal extraction with Benex*II step by step: Soft tissue, 12 weeks after extraction



Picture 5 Longitudinal extraction with Benex II step by step: Alveolar ridge, 12 weeks after extraction


Extraction System Ben**ex**[®]II acc. to Dr. med., med. dent. Benno Syfrig Polygon of forces, Polygon of forces conventional: with Benex*II: Pressure on the Purely axial traction alveolar wall by forceps or root elevator

All CE marked products according to the Medical Device Directive 93/42/EEC

are mentioned in the index from page 11-07.

In modern dental treatment, implantology following extraction is increasingly favoured. Consistent with the principle of minimal invasion, conserving soft and hard tissue structures is a must. Starting with extraction. The modified Benex II guarantees a gentle and simple extraction of roots in the whole mouth. It is nearly impossible to harm the soft tissue and the surrounding bone. Due to the longitudinal extraction, Benex IIis an optimal basis for direct implantation. It is also a valuable help for retarded implantation after the extraction with the Benex ${}^{*}\Pi$ system. Studies made after the use of $Benex^*II$ prove that the reossification of the extraction alveole is advancing optimally. This is a great advantage for the retarded implantation.

The new $Benex^*II$ is now available in a washbasket complying with the RKI guidelines. That way, the requirements of optimal cleanability and sterilization were taken into account. You will find further information, application examples and the Benex[®] user forum at: www.benex-dent.com



12.302.00 Benex[®]II Extraction System



zepf-dental.com

Extraction 05-03

Ratchet with demountable handle

Alveolar Ridge Preservation with Benex®

What does it mean?


Alveolar Ridge Preservation means the treatment of the dental alveolus after extraction. 3 months after the **Benex**^{*} extraction you find a considerably better ridge relation than with conventional gentle extractions. The **Benex**^{*} finds its successful application in both, private practices and universities. The **Benex**^{*} has achieved an

excellent status worldwide as basis for a subsequently successful implantation.

The new support for the dismounted $Benex^*$ System in a washbasket guarantees an optimal cleanability of $Benex^*$ in a washing machine or in an ultrasonic bath. All components can be fixed safely in the support.

Upon cleaning, the system can be sterilized in assembled condition.

In addition to the **Benex**^{*} components, an optional periotome, an Xtool and an optional **Benex**^{*} Pole Extractor can be placed in the support.

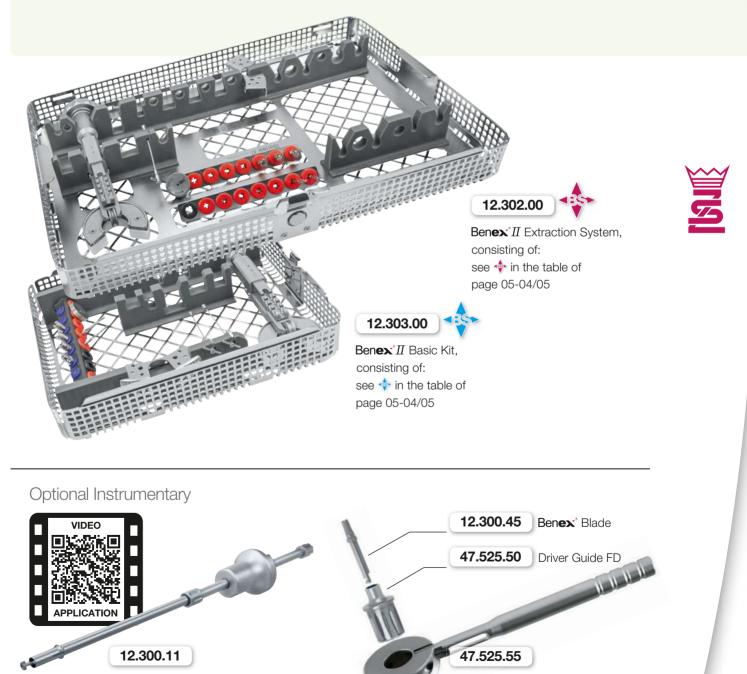

Benex* Pole Extractor

05-04 Extraction

05

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0

Illustration	Article Description	Order Quantity
	12.302.00 Benex*II Extraction System, consisting of:	1 piece
Marine Marine Marine	 Benex[*]II Extractor, 2 Pullropes 48 mm, Driver Guide, Screw short 1.6 mm + 2.1 mm, Screw long 1.6 mm + 2.1 mm, 1 Drill ea. for 1.6 mm, 2.1 mm Screws, Quadrant Support, 85.195.10 Washbasket with Lid, 	
	12.302.01 Tray/Rack for Benex II	
	12.302.01 Вел ех * <i>П</i> Tray / Rack	1 piece
	85.195.00 Washbasket 1/1 with Lid and Press Button Lock	1 piece
	 12.303.00 Benex[*] II Basic Kit, consisting of: Extractor, 2 Pullropes 48 mm, Driver Guide, Screw short 1.6 mm + 2.1 mm, Screw long 1.6 mm + 2.1 mm, 1 Drill ea. for 1.6 mm + 2.1 mm Screws, Quadrant Support, 85.194.10 Washbasket with Lid 	1 piece
*	85.194.10 Washbasket 1/2 with Lid and Press Button Lock	1 piece
**	12.300.08 Ben ex * <i>II</i> Extractor	1 piece
	12.300.15 Replacement Support Disc, 8 mm (PTFE), optional	1 piece
6	12.300.16 Support Disc, diagonally right, optional	1 piece
e de la companya de	12.300.17 Support Disc, diagonally left, optional	1 piece
**	12.300.20	2 pieces

K2019-03/1-E C C E All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

llustration	Article Description	Order Quantity
4.	12.300.30	2 pieces
	Diamond coated Drill for Screws Ø 1.6 mm 12.300.60 and 12.300.70	(1
and the second se	12.300.35	2 pieces
	Diamond coated Drill for Screws Ø 2.1 mm 12.300.65 and 12.300.75	(1 💠 💠)
*	12.300.47	1 piece
	Driver Guide, short	
	12.300.60	2 pieces
5	Screw, Ø 1.6 mm, 10 mm, S = Short	(1 💠 💠)
	12.300.65	2 pieces
	Screw, Ø2.1 mm, 10 mm, SF = Short & Fat	(1 💠 💠)
4	♦ 12.300.70	2 pieces
5.4	Screw, Ø1.6 mm, 16 mm, L = Long	(1 🐟 💠)
E.A.	12.300.75	2 pieces
	Screw, Ø2.1 mm, 16 mm, LF = Long & Fat	(1 💠 💠)
*	12.300.80	1 piece
	Quadrant Support for Benex [*] to bridgeover bigger gaps and for the universal molding	
and the second s	12.300.11	1 piece
N. Contraction of the second s	Benex* Pole Extractor, optional	
	47.525.55	1 piece
	Ratchet with demountable handle, optional	
	47.525.50	1 piece
	Driver Guide FD, optional	
	12.300.45	1 piece
	Benex * Blade for Driver Guide FD, optional	

Extraction 05-05

05

All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E







Application of the Extraction System

1. Anaesthesia. Cutting periodontal fibres (Sharpey fibres) in the sulcus by using the Periotome or the **HELMUT ZEPF** Nod.

2. Strong, large roots must be loosened / luxated by axial movements within 30 sec., using a slim elevator / twister (Xod from HELMUT ZEPF). Without using transversal movements. In case of multi-rooted teeth, the roots are divided and extracted separately.

3. Drilling with the diamond coated twist drill should be in the axis and center of the root fragment. It should be approx. 7 mm in the hard tissue, deeper drilling will not be necessary. Drilling is performed with water-cooling. In order to remove drilling chips more easily, an inward and outward movement is recommended for deep drilling.

Recommended rpm: 500 - 700 rpm REF 12.300.30 max. 3000 rpm REF 12.300.35 max. 2200 rpm

4. According to circumstances, the short or long extraction screw with screwing support **EF 12.300.47** is inserted.

5. The extractor is positioned on the adjacent crowns: The opening of the round, revolvable segment plate is adjusted in vestibular direction ensuring a good view of the extraction screw. After the pullrope has been hooked into the extraction screw, it is guided over the reverse roller and fixed to the hook of the extraction slide. Under slight traction - so that the rope does not hang out - the instrument is placed on the adjacent teeth by turning the hand screw. During positioning it is important to see that both the screw and the rope do have the same axial direction.

6. Once the extractor is positioned properly, the extraction is carried out by turning the hand screw. In case of strong, long roots the periodontal fibres have to be pre-stretched during 30 seconds by applying a sub-maximum traction.









zepf-dental.com



Dr. Maty Design

The exclusive design and 25% reduced weight make the *the cisica*-Instrument-Line light as a feather.

Extraction 05-07

The ergonomic handle design enables uniform power transmission during pressing, pulling and rotary movements and is equally suited for both right handed as well as left handed practitioners. The unique tip design adapts exactly to the tooth and is beyond comparison to other instruments.

The smooth handle with circular openings makes the *terr* Cisim -Instrument-Line extraordinarily easy to be cleaned since there are no more hygiene-critical zones as with instruments with serrated handles.

The ideal handling and tactual sensation is guaranteed.

From design to functionality, this product line answers all your concerns. The ^{TEPF} ★ *Cisi*() Handle is a registered model of **HELMUT ZEPF**, which has been developed with Dr. Maty.

6



05-08 Extraction

+49 (0) 74 64 / 98 88 0

Extracting Forceps



Pattern

All figures from **HELMUT ZEPF** are available in the **X***isi* Pattern



Diamond-Coating

All extracting forceps are available with diamond-coating for better grip. For ordering etc. just add to the item number the letter **D**.



Teflon Disc

The wear-resistant Teflon Disc eliminates wear and tear in the joints and provides a light action at all times.




Grooved Gripping Surfaces

Grooved gripping surfaces provide a secure grip and prevent slipping.





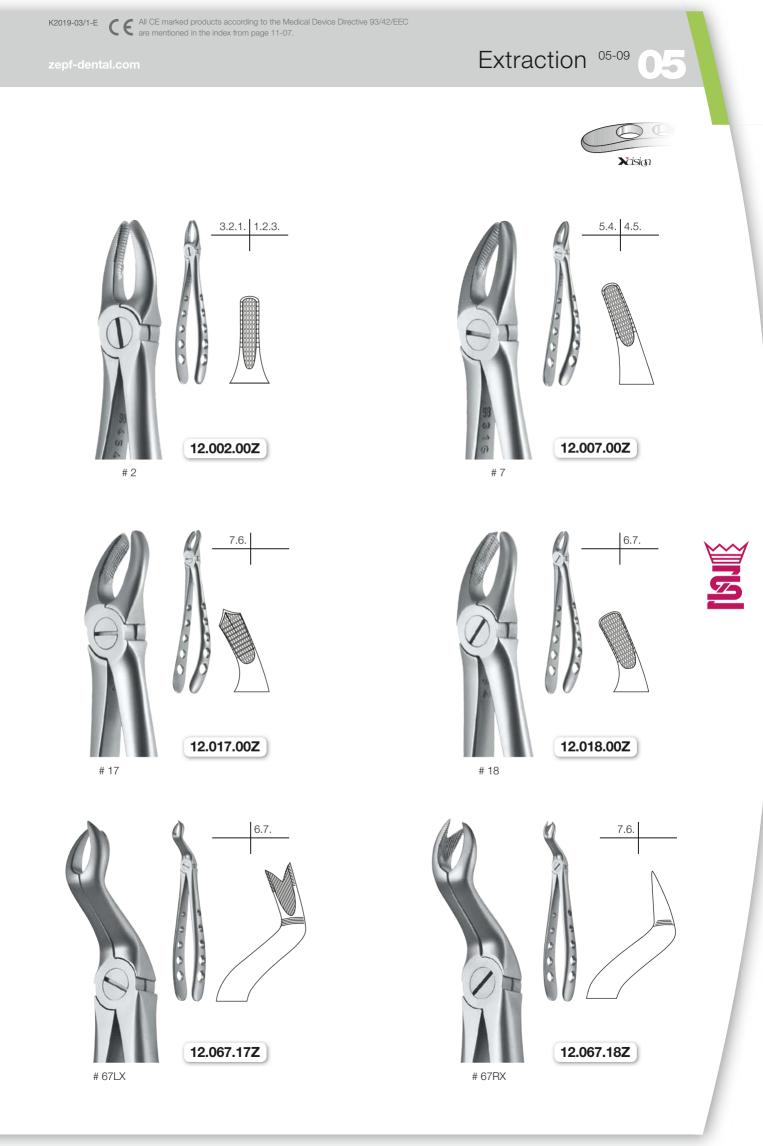

05-10 Extraction



1-





12.073.01Z

The slim, compact design of these **TEPF** Cisim Extraction Forceps allows easy accessing molar areas, even when mouth openings are restricted.






67A

12.067.01Z

8. 8.



51A



W





All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁵⁻¹² Extraction



0.5







3.2.1. 1.2.3.

34








34A



35

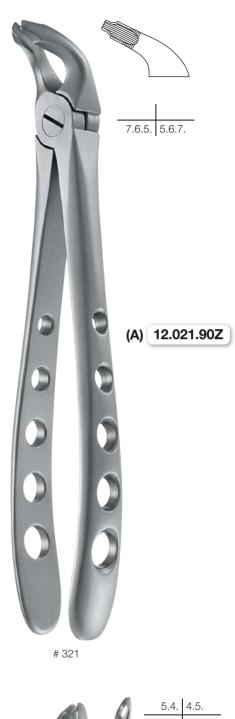





⁰⁵⁻¹⁴ Extraction

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

9 (0) 74 64 / 98 88 0



Secure-Line

Our special **HELMUT ZEPF** Extracting Forceps in our modern **TEPF X** *isi*(*s*) Design have tapered jaw tips. Their fine, sharp tips which have been anatomically shaped to match perfectly the teeth and allow to reach deep and large contact areas, which in turn provides better mechanical advantages and a more secure grip. Since these special **HELMUT ZEPF** Extracting Forceps have been designed for performing luxations, they have longitudinal grooves only on their jaws' gripping surfaces. The easy handling and superior "feel" of all our **TEPF X** *isi*(*s*) Lines of Extracting Forceps are of prime importance for this product line!



CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

Rescue-Line

No reason to panic! These forceps will allow you to carry out any extraction and work more efficiently even under complicated circumstances. If teeth break during extraction, these are the tools you need to rapidly, safely, solve your problems.


These forceps have special all-purpose jaws designed to cover a broad range of applications and have sharp pointed tips that allow separating the tips of roots from surrounding tissue by slightly twisting them and then securely trapping the extracted roots in the gaps between their jaws. The article numbers of extracting forceps with serrated edges are amended by 'ZS'.





12.051.15Z

12.051.15ZS

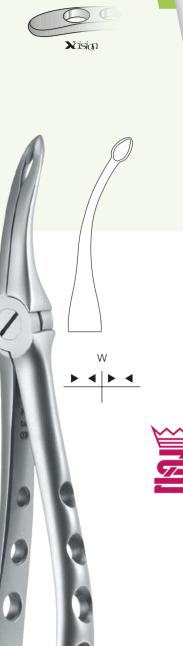

44Z

Extraction 05-15

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

05-16 Extraction

+49 (0) 74 64 / 98 88 0



Special Wisdom Routurier Extracting Forceps

Their angled shape will allow you to reach around obstacles and protect the corners of patients' mouths whenever their mouth openings are restricted or their jaws have been firmly clamped in position. Their slim compact design allows readily accessing molar areas.

Witzel All-Purpose Root-Splinter Forceps diamond-tipped

Our special forceps for extracting root splinters from both upper and lower jaw have diamond-tipped jaws for the best possible grip, and are the ideal complement to our Rescue-Line.

If their diamond tips should ever become worn, simply contact our retipping service, who will put new diamond tips on them for a fixed charge.













⁰⁵⁻²⁰ Extraction

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

(0) 74 64 / 98 88 0

Extracting Forceps, American Pattern

Diamond Version


All forceps are also available in the diamond version. For ordering etc., just add a ${\bf D}$ to the article number







zepf-dental.com




Extracting Forceps, American Pattern




0.5

Extracting Forceps, American Pattern

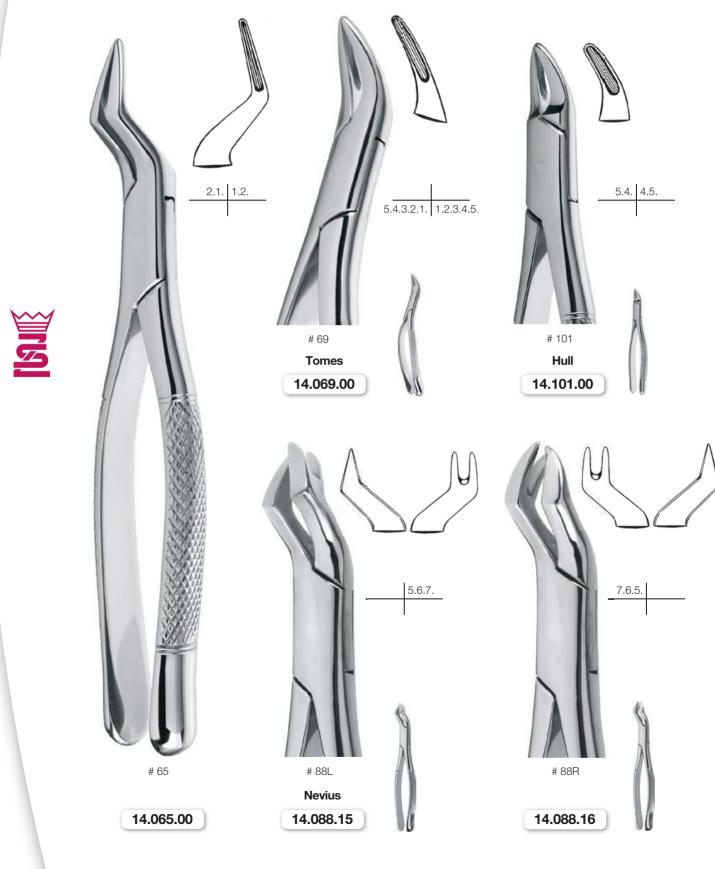

zepf-dental.com



Extracting Forceps, American Pattern




⁰⁵⁻²⁴ Extraction

0-5

+49 (0) 74 64 / 98 88 0

Extracting Forceps, American Pattern



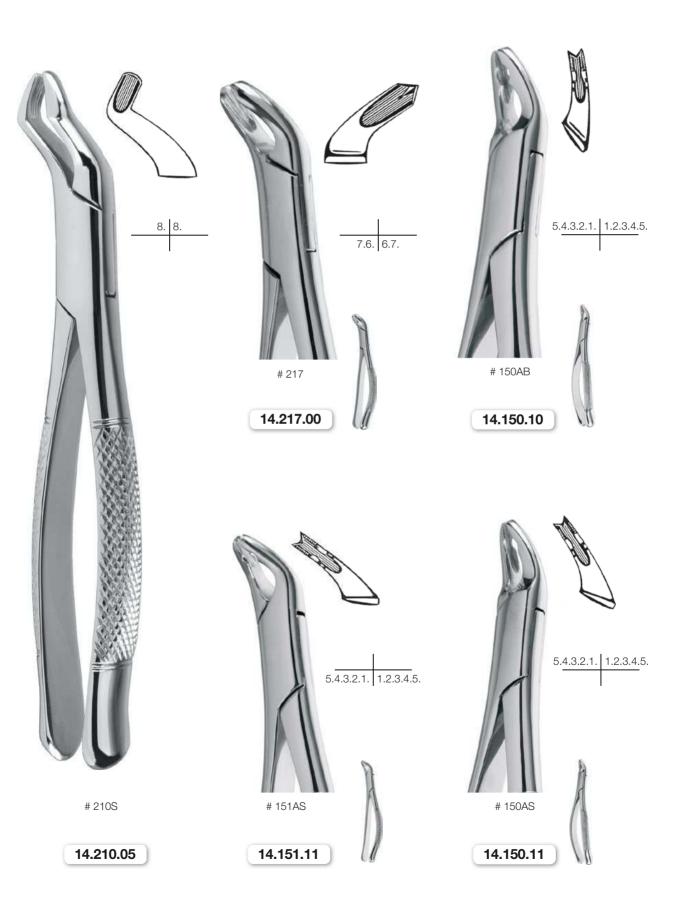


zepf-dental.com

Extracting Forceps, American Pattern

Extraction 05-25

0.5

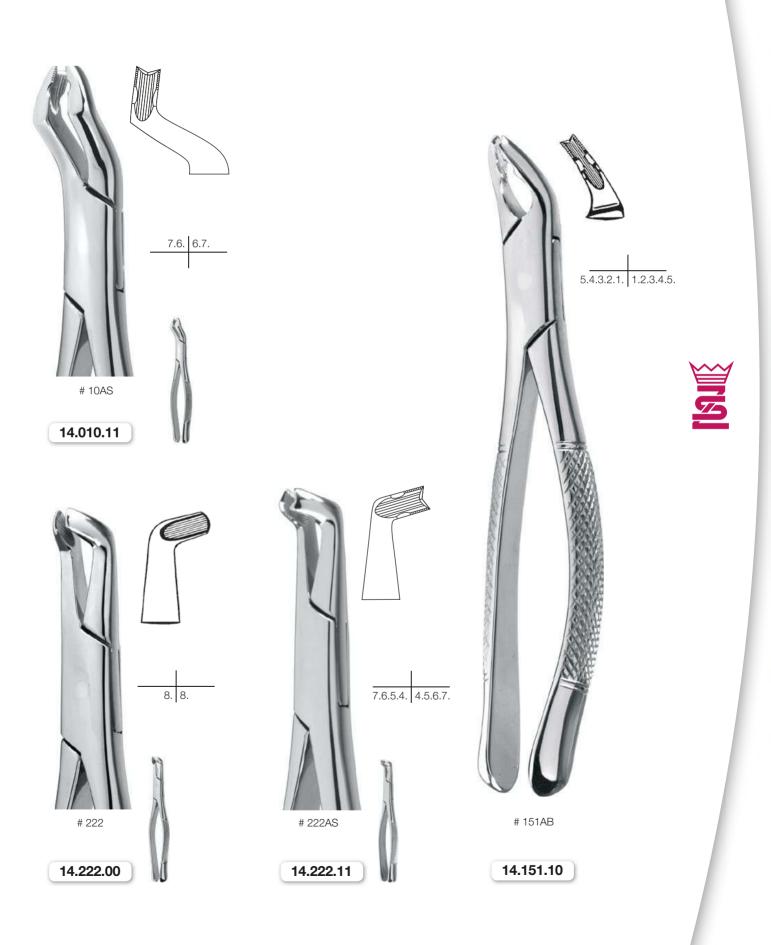


⁰⁵⁻²⁶ Extraction

+49 (0) 74 64 / 98 88 0

Pedodontic Extracting Forceps

These pedodontic extracting forceps have been designed to be as small as possible in order to avoid frightening younger patients with large, aggressive-looking instruments, thereby providing relaxed working conditions.

Further RoBa-Design Pedodontic Extracting Forceps are illustrated on page 05-32!

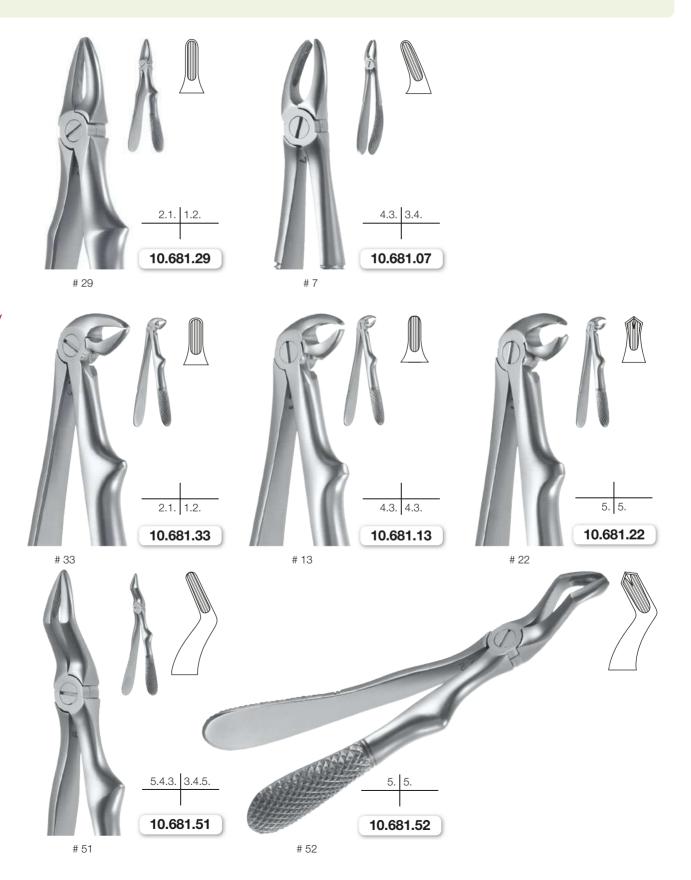

zepf-dental.com

ZEPF



Extraction 05-27

ZEPF RoBa-Edition by dentist Beck

Dedicated to the long-standing employees Mr. Horst Roos and Mr. Reinhold Bacher, who worked for Helmut Zepf for more than 50 years since their time as trainee.

The **ZEPF** RoBa-Edition completes the innovative advancement of the famous **ZEPF C***isi* **(**) Extracting Forceps. It has been developed under the aspects of a secure and gentle appliance.

The problem of tooth fractures during extraction is considerably reduced due to the innovative geometry of the beaks.

The new ONYX coating makes the impact-resistant surface of these extracting forceps almost indestructible.

Compared with other methods, in ONYX coating the carrier material is applied in a more gentle way, as ONYX coating in comparison to other coatings is performed with significantly less influence of heat.

The surface shows excellent sliding features to reliably counteract contamination. An incrustation of proteins etc. is not possible.

The matt-finished black surface not only prevents reflection of the OT light, but also guarantees an optimal contrast in the OR environment during extraction. All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0


ZEPF E D I T I O N PATENTED

With the patented RoBa-Edition **HELMUT ZEPF** introduces a new generation of extracting forceps. Deduced from the **TEPF X***isi*(*t*) Instruments the RoBa-Edition has been especially developed in consideration of easy and gentle extraction.


The patented RoBa-Edition according to Dentist Beck is the consequential advancement of conventional extracting forceps with the advantages of the tapered deep-grip extracting forceps. The modified beaks according to Dentist Beck fit exactly on the teeth which ensures a maximum grip in the appliance. These new beaks are available for all figures in upper and lower jaw (incisors, premolars, molars and wisdom teeth).

Due to the fact that all teeth show a convex crown contour (upper jaw: labial, buccal, palatal and in lower jaw: labial, buccal, lingual), the beaks have been developed under this anatomical conditions The handle is a protected design from **HELMUT ZEPF**, which was developed in co-operation with Dr. Maty, Germany.





- (1) The serrated jaws grip onto into the teeth and avoid a "riding" in-between the tooth crown and the inner contour of the beak.
- (2) Concavely elaborated inner contours of the forceps beak fit in the convex tooth contour. With deep grip in the alveolus on the neck of the tooth or on the crown, the RoBa Edition ensures a parallel and maximum grip in any situation. Root fracture almost can be excluded.



- (3) The different deeply elaborated inner contours ensure maximal adaptation on the teeth in different actualities. No tilting of the teeth while rotary and / or lifting movement.
- (4) Tapered outside contour of the beak affords deep grip even subgingival.

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Extraction 05-29



Black Finish Coating

Design meets functionality.

Users with highest demands will appreciate the elegant, black finish providing the instrument with a non-reflecting, extremely smooth and scratch-resistant surface. The article number is complemented by **TI**.





Diamond Version

All RoBa-Edition extracting forceps in the classic satin-metallic finished surface are available with diamond coating for a better grip.


The lower part of the **TEPF** Cisic Handle is gold-plated. For ordering etc., just add a **D** to the article number.



05-30 Extraction

12.236.08ZD

12.236.08ZTI

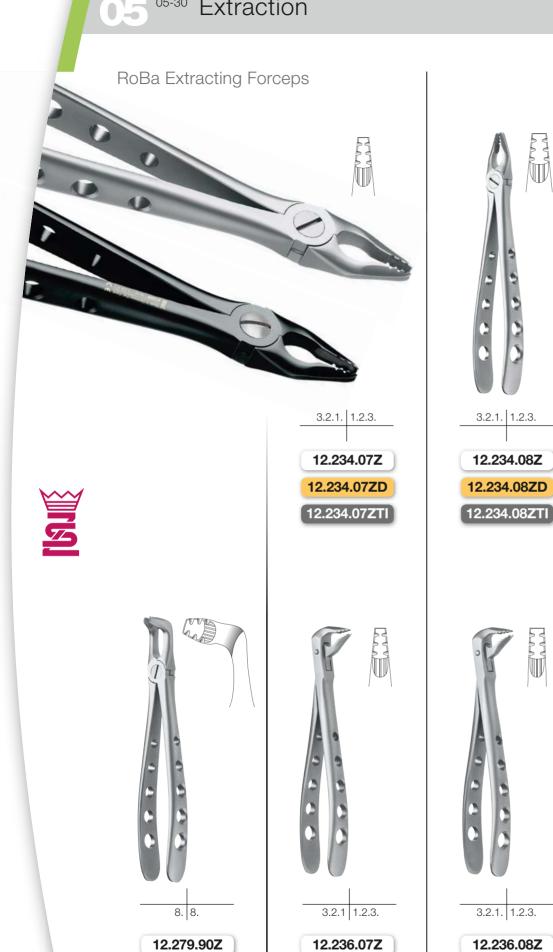



12.279.90ZD

12.279.90ZTI

12.236.07ZD

12.236.07ZTI

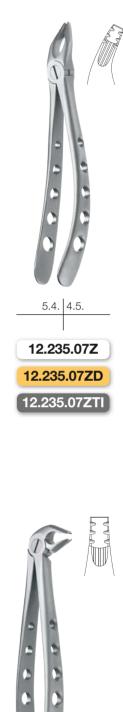



K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

Extraction 05-31



S

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁵⁻³² Extraction

+49(0)7464/98880

Children Forceps RoBa-Edition

Extracting Forceps modif. by Dentist Beck

These deciduous teeth extraction forceps have been designed to be as small as possible in order to avoid frightening younger patients with large, aggressive-looking instruments, thereby providing relaxed working conditions.


The patented Deciduous Teeth RoBa-Edition Forceps according to Dentist Beck are the consequential advancement of conventional extracting forceps with the advantages of the tapered deep-grip extracting forceps. The modified beaks according to Dentist Beck fit exactly onto the teeth which ensures a maximum grip during the appliance.







4.3. 3.4. 10.685.13



22



51



The wear-resistant Teflon[®] disc eliminates wear and tear in the joints and provides a light action at all times. **K2019-03/1-E C C E** All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

04.0

0.0

Refreshingly Innovative

The new generation of extracting forceps in the patented **ZEPF exlo** Design was designed to meet the special requirements of gentle removal of teeth. To meet these requirements, we composed a programme of 11 extracting forceps figures out of more than 400 existing figures. These were chosen according to anatomy, ergonomics and hygiene.

Extraction 05-33

Pat. U.S. 7,318,725 B2

exlo





3.2.1. 1.2.3.

15.034.01

34A







0-5

 \mathbb{U}

ex

(6

34

3.2.1. 1.2.3.

15.034.00

The exLG Forceps offer an excellent anatomic fit and only need enough pressure so they do not slip out of the hand. The forceps guarantee a balanced axial luxation, better periodontal fibre dilatability and increased sense of touch. They reduce traumata of surrounding tissue.

The assimilated handles allow an individual and equal power transmission for left- and right-handed surgeons during pressing, pulling and turning movements.

Due to the smooth handles and the possibility of dismantling, the **exlog** Forceps can be cleaned extremely well. So there are no hygiene-critical areas any more like they are known from forceps with conventional lock. Especially with automatic reprocessing in a washtray the disassembly is a great advantage as they need less space.



36

36A

21N

Extraction 05-35

-



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁵⁻³⁶ Extraction

+49 (0) 74 64 / 98 88 0

All Advantages on One View:

- excellent anatomic adaptation on the tooth surface
- tapered beaks for less trauma and protection of the alveolar loculus
- linear serrated jaws for equal axial luxation
- better fibre dilatability and increased sense of touch
- optimal cleaning through the demountability of the forceps into two parts (RKI-compliant)
- long lasting, patented, high precision joint for radial and axial mechanical load
- made out of one piece (5-axis CNC-milling) for ultra high precision
- no maintenance of the joint necessary

Focus on the exl_G , the standard of tomorrow.

A NEW STANDARD IS DEFINED



K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

ZEPF

Ε

PATENTED



ZEPF EXLOG RoBa Edition Extracting Forceps

Extraction 05-37

With the new **exlog** RoBa Edition **ZEPF** introduces a new generation of patented extraction forceps. Two patented extraction forceps are combined into one.

The EXLOG Forceps characterized by the fact that it's easy to disassemble and the RoBa characterized by its patented jaws.

It made sense to combine both patents as the combination results in a type of forceps which is easier to clean than ever before and additionally offers the dentist a functional extraction tool which leaves no desire unfulfilled.

These patented forceps are the consequent development of conventional forceps with the advantage of tapered and deep grip extraction forceps. The modified jaws exactly match the tooth and guarantee a maximum grip during the application.








K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

Extraction 05-39

3

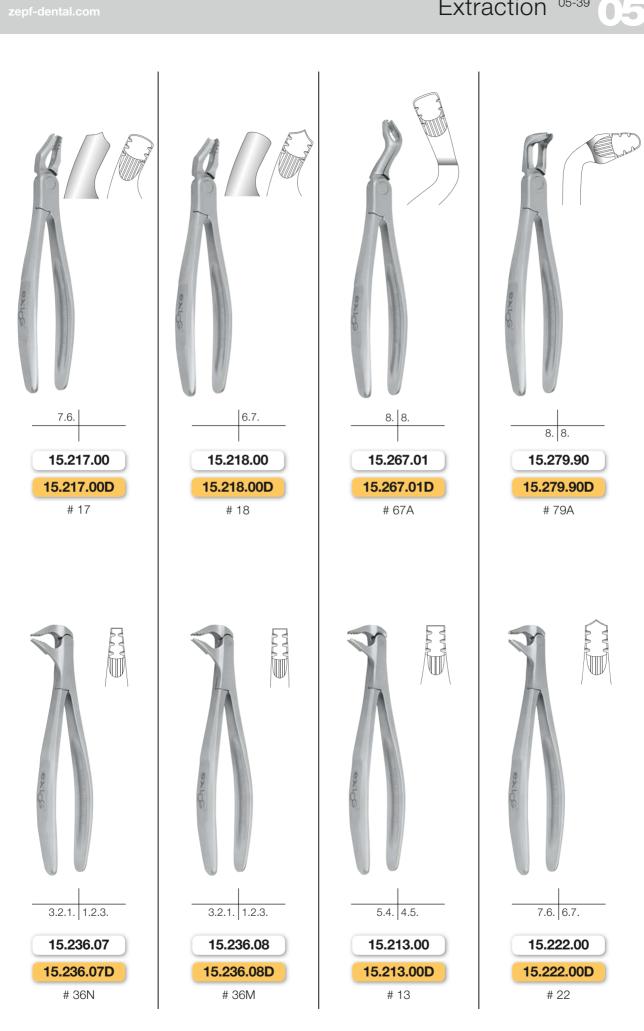

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

05-40 Extraction

+49 (0) 74 64 / 98 88 0



ZEPF

F


ZEPF EXLOG RoBa Edition Extracting Forceps

This new development involves all figures for maxilla and mandible (incisors, premolars, molars and wisdom teeth).

As every tooth shows a convex crown shape (maxilla: labial, buccal, palatal – in the mandible: labial, buccal, lingual), the jaw was developed according to these anatomical conditions.

- excellent anatomical adaption on the neck of the tooth surface
- tapered jaws for less traumatization and for conservation of the alveolus
- better fibre dilatability and increased sense of touch
- optimal cleaning due to the possibility to disassemble the forceps into two pieces (RKI compliant)
- Iong life time, patented, high precision joint for radial and axial pressure
- produced from one piece (5-axis CNC milling) and therefore ultra precise
- no maintenance of the joint





PATENTED

The following problems might occur if the extraction forceps are not suitable:

- root fracture
- crown fracture
- damage of the soft tissue caused by bruising
- damage of the alveolar ridge and the buccal bone lamella



Advantages of deep-grip extraction forceps:

- due to the specially shaped jaws it is easy to place the forceps subgingivally directly on the root (below the gingival margin)
- parallel contact on the root
- atraumatic, as the soft tissue is not bruised
- root fractures are avoided
- slim jaw design for subgingival grip without bruise of the soft tissues

zepf-dental.com

Extraction 05-41

THE ORIGINAL

DBGM acc. to Dr. Dettef Hildebrand



Xtod Instruments







17.007.01

In the illustrations an extraction under use of the λtod Instruments is shown.

IMPORTANT: Complete removal of all inflammable and convective tissue structures.

- Initial loosening of the desmodontal fibres. Apply the X-Desmo-Tool first approximally then buccally and palatinally (pencil handle).
- (2) Then progressive luxation with the X-Luxa-Tool (first narrow then wide). Ideal positions: Approximal (mesial or distal) to the tooth which should be extracted!
- (3) Complete luxation of an upper right molar with support of a wide X-Luxa-Tool. Gentle extraction without root fractures!
- Inspection of the empty tooth socket and curettage with support of the X-Spoon.



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁵⁻⁴² Extraction

+49 (0) 74 64 / 98 88 0

Xtod Instruments DBGM by Dr. Detlef Hildebrand

THE ORIGINAL


The implantology with immediate insertion after the tooth extraction is more and more a focus of interest in modern dentistry. It appears to be more than necessary to protect soft and hard tissue structures already during the extraction phase and to follow the principles of minimal invasiveness. Here is an ideal complement for this:

The Xiod Instruments! In contrast to existing instruments this clearly arranged and universal Xtool Set supports you during the gentle and uncomplicated extraction of teeth which cannot be preserved.

Modern therapy methods require modern instruments!




- Color coding for clear handling.
- Universal and complete extraction instruments in one tray.
- Ergonomic handle design (pencildesign) prevents unintended slipping during usage.
- Direct and controlled power transmission to prevent tooth and root fractures.
- Non-traumatic tooth extraction without injuring surrounding structures.



Design meets functionality.


Users with highest demands will appreciate the elegant, black finish providing the instrument with a non-reflecting, extremely smooth and scratch-resistant surface. The article number is complemented by **TI**.



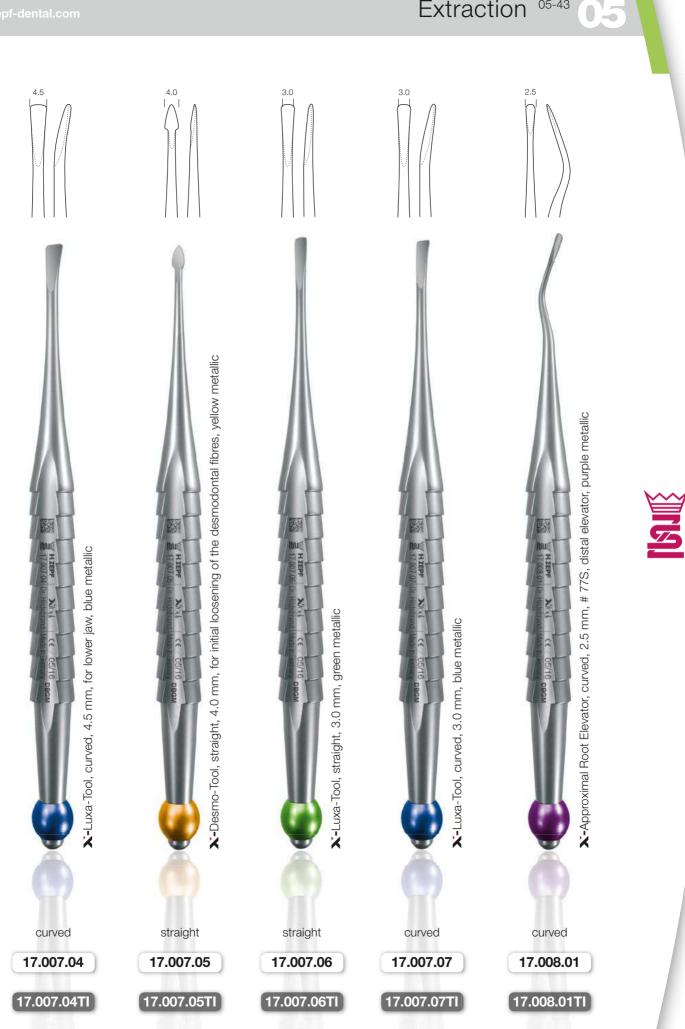


05-44 Extraction

5

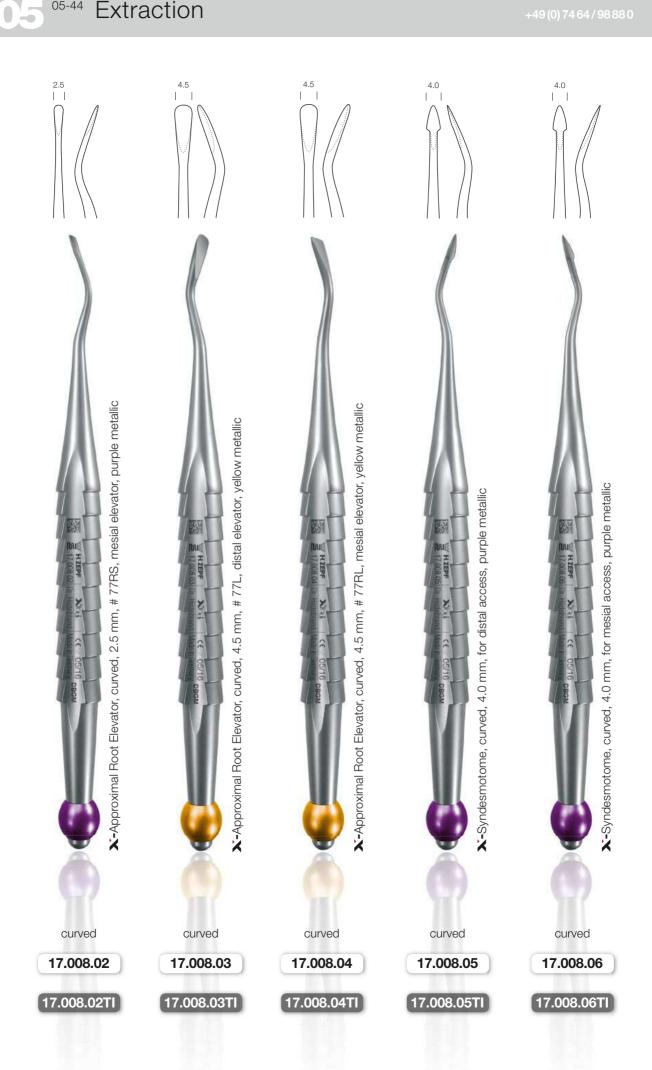



Extraction 05-45

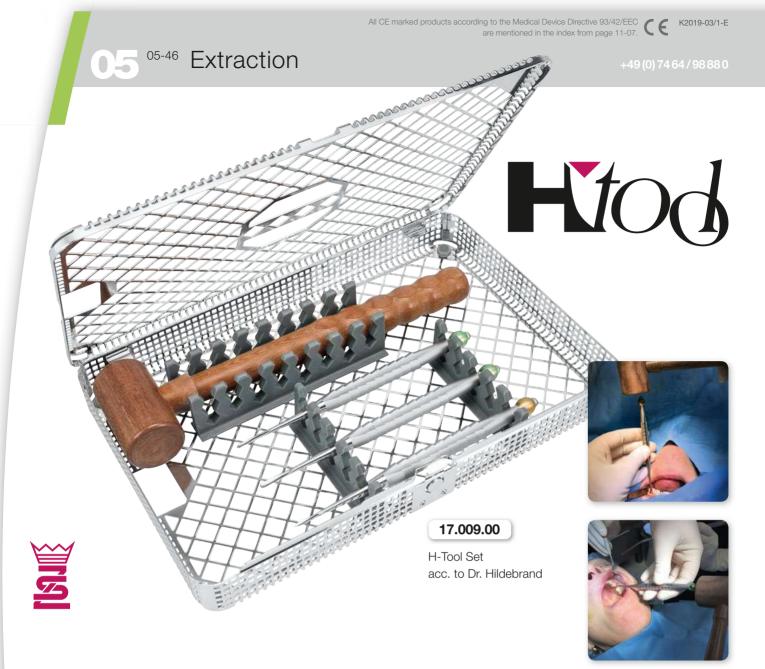



The new H-Tools developed by Dr. Hildebrand are a continuation of the successful X-Tool concept. The instrument tips are very flat and

sharp pointed. The instruments are inserted along

the root axis and the alveolar cavity is widened by advancing the H-Tool apically along the root of the tooth to be extracted with gentle hammer blows.

The light ferrozell hammer with a diameter of 35 mm enables work to be carried out safely.

Thanks to the extremely light construction, this hammer produces a far less unpleasant feeling in the patient than using a hammer with hard plastic inserts or in the worst case with a metal head.



K2019-03/1-E C C E All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

Extraction 05-47

0.5

Content: H-Tool Set

llustration	Article Description	Description
	17.009.00 H-Tool Set by Dr. Hildebrand organized in a washbasket, including a Ferrozell hammer and H-Tools, consisting of:	Complete set
	41.503.01 Hammer, Ferrozell head Ø 35 mm, 100 g, total weight 180 g, 250 mm long, fitting washbasket	1 piece
E 1785 Sul and su	17.009.01 H-Tool # 1, straight, tip 3.5 mm, green ball	1 piece
E 1920 hu inclusion	17.009.02 H-Tool #2, straight, tip 2.5 mm, green ball	1 piece
S INT. W LICHW II	17.009.05 H-Tool #5, straight, tip 3.0 mm, gold colored ball	1 piece
C C C C C C C C C C C C C C C C C C C	85.195.00 Washbasket 1/1 as rack for the remaining components	1 piece
	85.181.04 Profile, high, universal 130 mm / for 8 instruments	2 pieces
LEELEEL	85.181.05 Profile, high, universal 81 mm / for 5 instruments	2 pieces

05-48 Extraction

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0

ZEPF-Xtod-Tray

DBGM by Dr. Detlef Hildebrand

"Extraction in its most pleasant way"

The **ZEPF-X**od-Tray offers a universal instrument set for medical tooth extraction. The **X**od instrumentation includes six different instruments:



• X-Desmo-Tool (yellow): The X-Desmo-Tool easily penetrates into the periodontal gap with its pointed tip and initially loosens the Sharpey's Fibres. The modified pencil handle and the handy shaft shape offer a depth sensibility like never experienced before without

17.007.00

Complete Set consisting of

17.007.01 - 17.007.05 and 41.855.01Z in the washtray

X-Luxa-Tool-3 (blue):

destroying related structures.

bent + narrow for tooth loosening

X-Luxa-Tool-1 (green):

straight + narrow:

A delicate and controlled power transmission guarantees a specific loosening and luxation of the tooth without any risk of crown or root fractures. **Ideal position:** approximal (mesial or distal) to the tooth which is to be extracted.

X-Luxa-Tool-2 (green):

straight + wide:

Complete, non-traumatic luxation of upper molars (e.g. tooth 16). The ergonomic instrument shape ensures a gentle extraction without tooth fractures or any damage to the alveolar wall.

X-Luxa-Tool-4 (blue):

bent + wide: for tooth luxation

Lucas Schaber ZEPF-Line:

Inspection and curettage of the empty dental alveolus. Complete removal of all inflamed and connective tissue fibres.



ZEPF FLEX-EX Power Periotome



While using new materials, we were successful in the development of the **ZEPF** *FLEX*-EX Power Periotome, a symbiosis of Power Periotome, Elevator and Xtool.

The flexible working tip will enable you to build up a phenomenal pressure for the luxation in a radial direction and a perfect match to the contour of the tooth at the same time without bending. The name stands for the excellent product features united in this instrument.

ZEPF Power Periotome

The Power Periotomes allow a gentle loosening of ligaments in the sulcus. The handle allows optimal power transmission and controlled luxation.



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.


⁰⁵⁻⁵⁰ Extraction


+49 (0) 74 64 / 98 88 0

Ergonomical and heavy

0.-5

Heavy, ergonomic handle design with exchangeable tips, for optimal access to all quadrants.

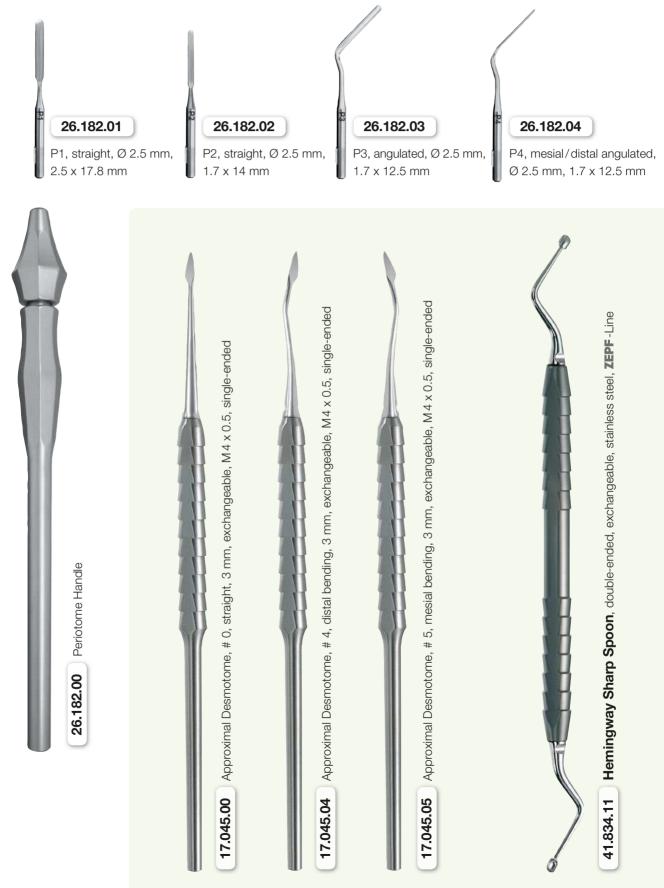

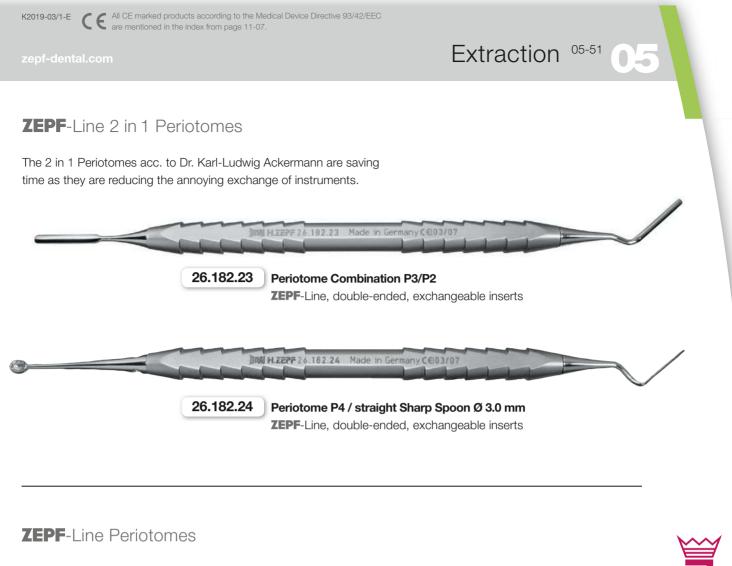

For the Separation of the Sharpey's Fibers in the Sulcus

Before the usage of any root elevator or extraction forceps it is necessary to separate the Sharpey's Fibers in the sulcus with a periotome in order to do an atraumatic tooth extraction. To do so, the periotome is to be pulled through the sulcus.

The correct application saves the gingiva and the periosteum. The special design in the grip area guarantees a pleasant grip and extremely easy handling.



⁰⁵⁻⁵² Extraction

3.0 mm

49 (0) 74 64 / 98 88 0

Root Elevators

Root elevators are used for the surgical tooth extractions. They are used to luxate the tooth in the osseous alveolus and to expand the alveolus walls. They are also used to open the gingival sulcus prior to the tooth extraction.

Straight instruments are used in the anterior region and in the maxillary area. Curved root elevators are ideal for the back teeth in the mandible.

The Workmanship

The shafts of **HELMUT ZEPF** Root Elevators are welded onto their hollow handles, and each and every one is checked for leakage at their welded joints.

This manufacturing method virtually eliminates the leakage compared to cheap root elevators with pressed-in shafts.



Bein

Bein

(B) 17.001.01

(S) 17.001.11

(B) 17.001.00


(S) 17.001.10



The Handle Versions

Except for the Xtool-Series, the Elevators from **HELMUT ZEPF** mainly differ in their 6 different handle designs such as: 'Bein', 'Carpal', 'Standard', 'Flohr', 'Mini'.

These are handle versions which can be assigned easily due to their letter coding:

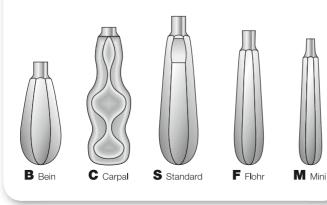










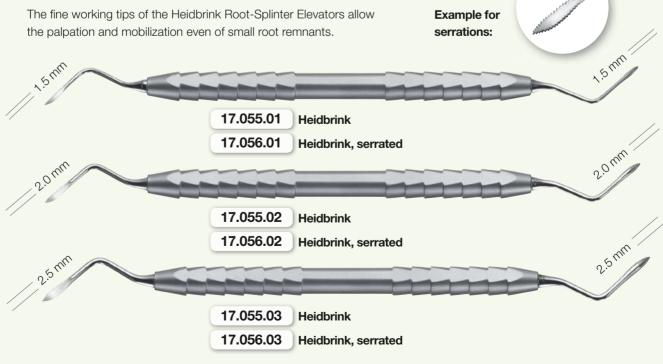

Root Elevator No. 195

The drop-shaped, blunt working end makes the new **ZEPF** Root Elevator No. 195 ideal for the separation and luxation of roots. The tapered working end allows its special use in the molar region in all quadrants. It can also be used for initial loosening of the desmodontal connection.

Due to its geometry and smooth luxation and rotary motion, the root fragment to be

T

removed will be moved very easily in "crestal direction" (in relative terms!). The luxated fragment can therefore be grasped easily with deep-gripping forceps or with Luer bone rongeur forceps.



Picture: Courtesy of Dr. Florian Steck

题

📜 🖪 Bein

🐌 C Carpal

S Standard

🗏 F Flohr

🕽 🖬 Mini

Extraction 05-55


(S) 17.195.00 Root Elevator No. 195



Lindo-Levien Root Elevators

The LINDO-LEVIEN Root Elevators are pushed into the periodontal gap in apical direction until the serrations will grip on the roots. The root is extracted via a barb effect by straight pulling without leverage.

	-	
4.0 mm	3.5 mm	3.0 mm
(S) 17.395.01 # LLL	(s) 17.395.02 # LLM	(s) 17.395.03 # LLS
4.0 mm	3.5 mm	3.0 mm
(S) 17.396.01 # LLLC	(s) 17.396.02 # LLMC	(s) 17.396.03 # LLSC

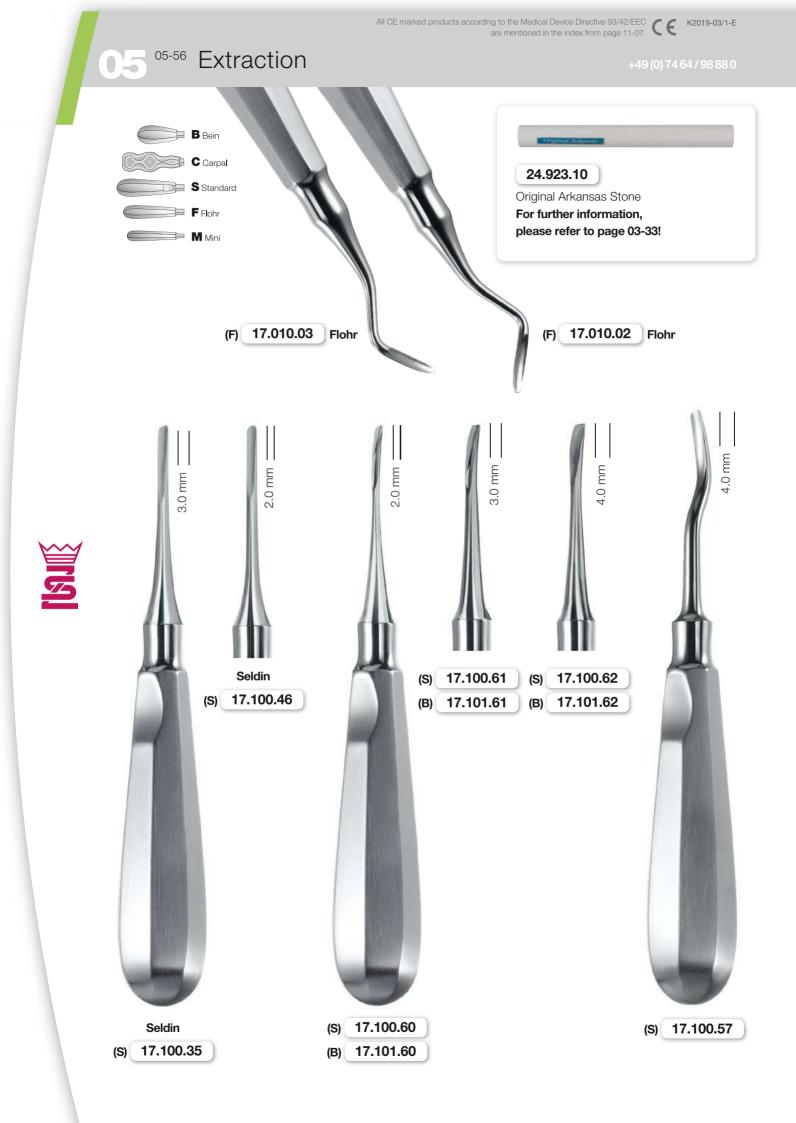

3.0mm .

17.100.08 Miller

(S)

zepf-dental.com

Extraction 05-57

(S) 17.100.11 Miller

3.0 mm

(S) 17.100.10 Miller

~ 3.0 mm

0 -5

. 3.0 mm

Elevators for axial luxation

These elevators for axial luxation have been developed as an alternative to classic elevators. The instrument must not be used as a lever.

Furthermore the gentle removal of the teeth should be reached by **axial luxation** and cutting the Sharpey's fibres.



(s) **17.006.01** straight

5.0 mm

straight

17.006.02

ŝ






17.100.09 Miller

ŝ







Technique for molars





17.410.03 Chompret Syndesmotome, # 3 with hollow handle






zepf-dental.com

Root Elevators Cryer and Winter

Claw elevators are ideal to extract molars in the mandible after separation of the roots.

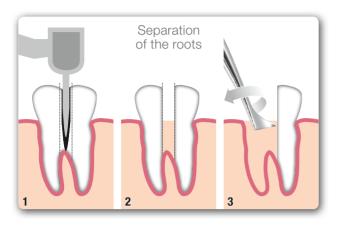


The bend of the working ends, combined with the shortened tips, allows a gentle lifting of the opposite root without contact to the neighboring crown.

The special claw elevators are ideal to luxate roots if an apical access is possible from the neighboring alveolus, e.g. if a root has already been removed and if the empty alveolus can be used as access. It is recommended first to remove the root which is bent less.





Extraction 05-61

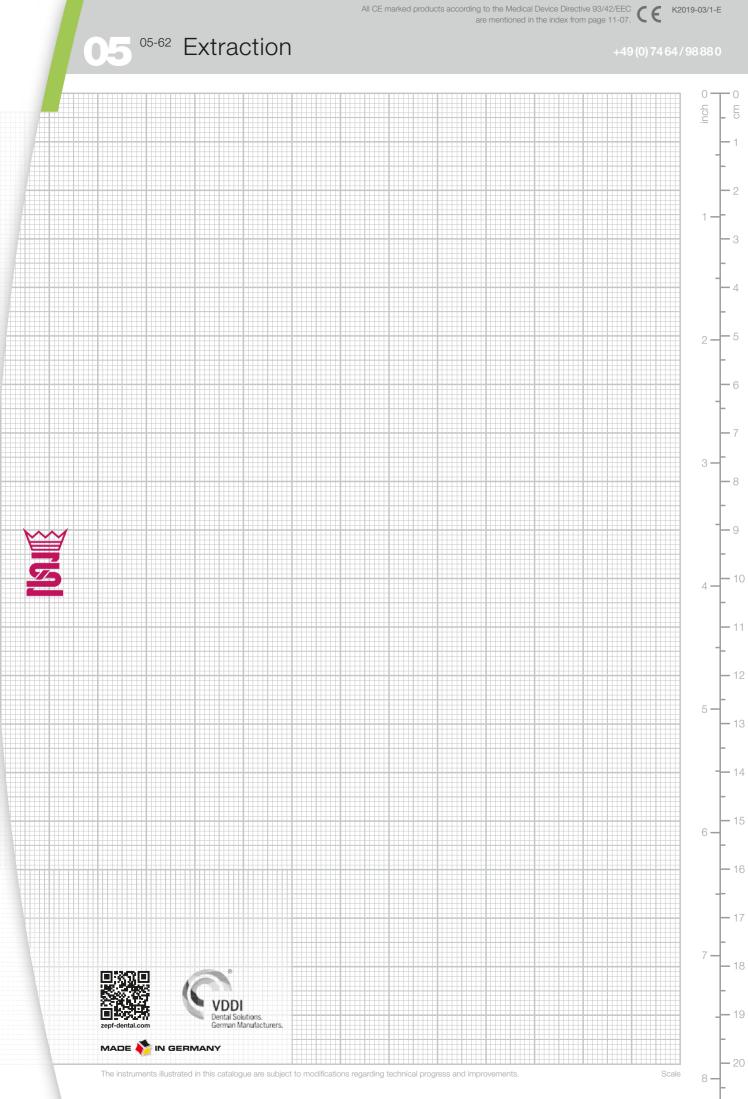

K2019-03/1-E

zepf-dental.com


Oral Surgery 06-01

HELMUT ZEPF Oral Surgery and Maxillofacial Instruments


INM H. ZEPF 19:551.15M Made


CEIDSI

This chapter for Cranio-Maxillo-Facial Surgery includes all instruments required for reconstruction of traumata, diseases, bone fractures, malformations and deformations of the teeth, the oral cavity and for the jaw as well as the face.

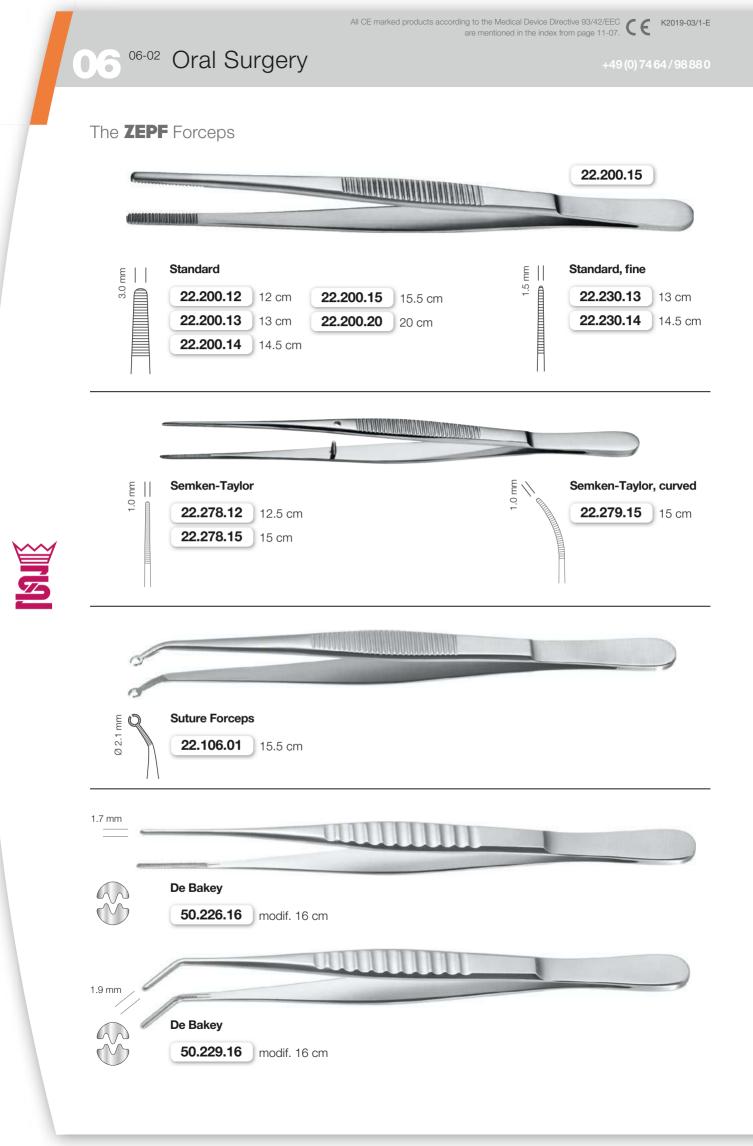



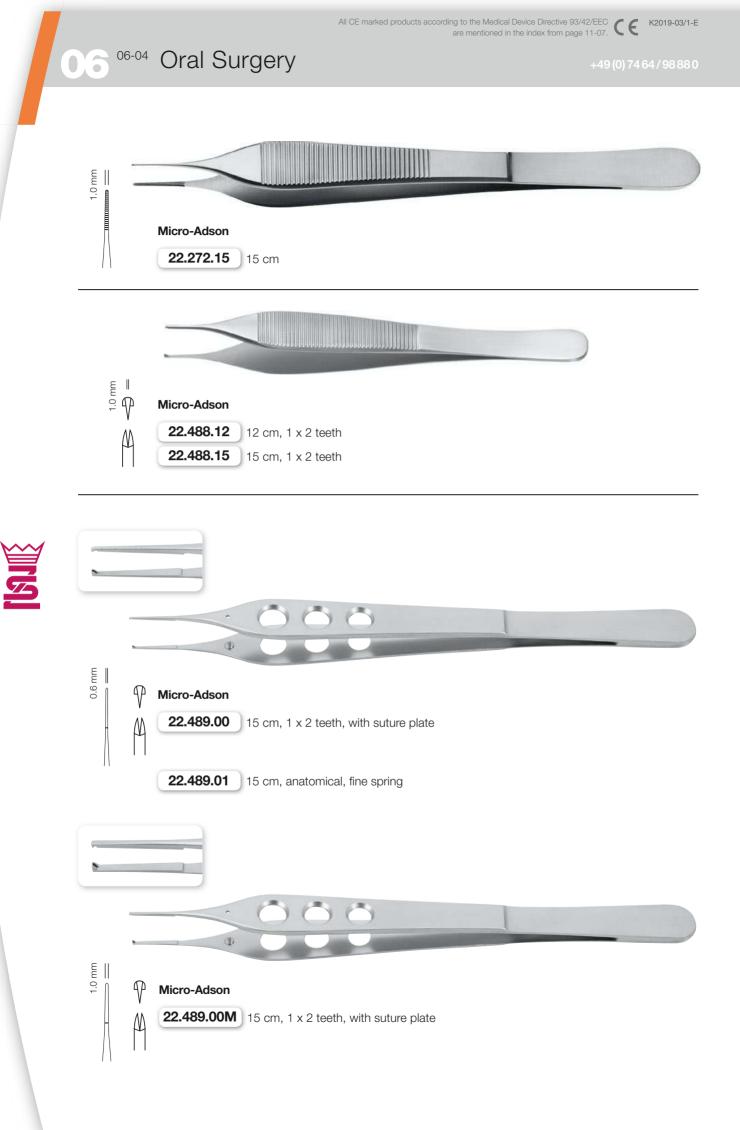

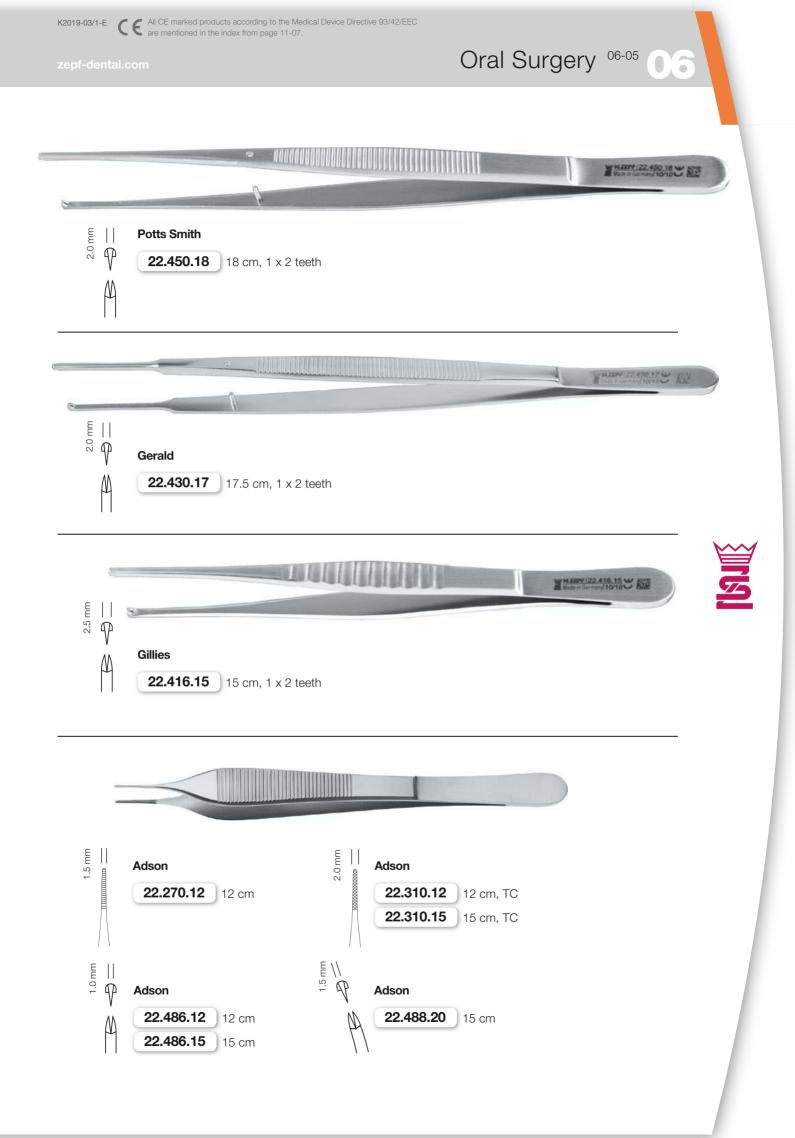







The **ZEPF** Retractor

pat. pend. by Dr. Peter Müller, Ebersbach



Clear, non-tiring retraction in every situation

Retraction of the cheek, lips, tongue and mucoperiosteal flap. The ZEPF Retractor is a "quality product from Tuttlingen" and bears the name HELMUT ZEPF as seal of quality.

- ergonomic handle
- low-weight, very well-focused instrument
- innovative design
- multipurpose usage
- good view
- smooth surface, manufactured from one piece
- all common disinfection and sterilization methods possible







37.445.01 Hilger Retractor, for all Mouth Mirror Handles Ø 2.5 mm

24.089.02 Mouth Mirror Handle, ergonomic, hollow, stainless steel



zepf-dental.com

Oral Surgery 06-09

016



Vestibulum Retractor acc. to Dr. Müller, Tuttlingen

Working end made of stainless steel, handle M 4.5 mm, Dr. Ti, made of titanium.

The Vestibulum Retractor acc. to Dr. Müller, Tuttlingen can be used in the dental field for all activities for which it is necessary to have a very good view as well as the best possible dryness.



The application in periodontology as well as in oral surgery is possible as the Vestibulum enables you to retract a complete quadrant. This offers a very good view on your field of work. The instrument can also be used to model the edges in the acrylic technique. The relative drying is possible with one hand which offers a better moulding.

The instrument can be used in many ways and is very easy to apply. This makes it very economical. 37.444.01

Igi

Maty Cheek and Lip Retractor

06-10 Oral Surgery

+49 (0) 74 64 / 98 88 0

Special features of the Maty Cheek and Lip Rectractors:

- suitable for a wide variety of applications
- lightweight
- easy to use
- patient-friendly

37.454.00

Maty Cheek and

Lip Rectractor, 17.5 cm

- no traumatization of the oral cavity
- usable on upper or lower jaws
- ergonomically designed, saves time, thereby cutting costs
- does not need to be removed when work is interrupted since design prevents the dropping out

jaws of this instrument makes it suitable for use in a wide variety of applications in all areas of dentistry.

In prosthodontics, for safe impression technique, determining upper/lower jaw mismatches, fitting crowns, bridges, inlays, etc

The light weight, versatility and anatomically shaped



- In orthodontics, for fitting brackets, etc.
- In general dentistry, for filling teeth, root-canal work, etc.
- In oral surgery, for outpatient surgery (apicoectomy, osteotomy, tumor and bone surgery, etc.), preprosthodontic surgery, traumatology, implantology (enossal implants, sinus lifting, GBR techniques, etc.)



Due to its diverse application possibilities and easy handling (no specialists required to retract lips, cheeks etc.) the retractor also contributes significantly to cost-efficiency.

Quality MADE IN GERMANY.

Our all-purpose cheek and lip retractor is yet another top-quality, high-precision, all-purpose instrument "Made by **HELMUT ZEPF** Medizintechnik GmbH".



Maty Cheek and Lip Rectractor for children




Oral Surgery 06-11

•



37.446.04

Retractor acc. to Kim, flat, 45° angled, 10.5 mm wide

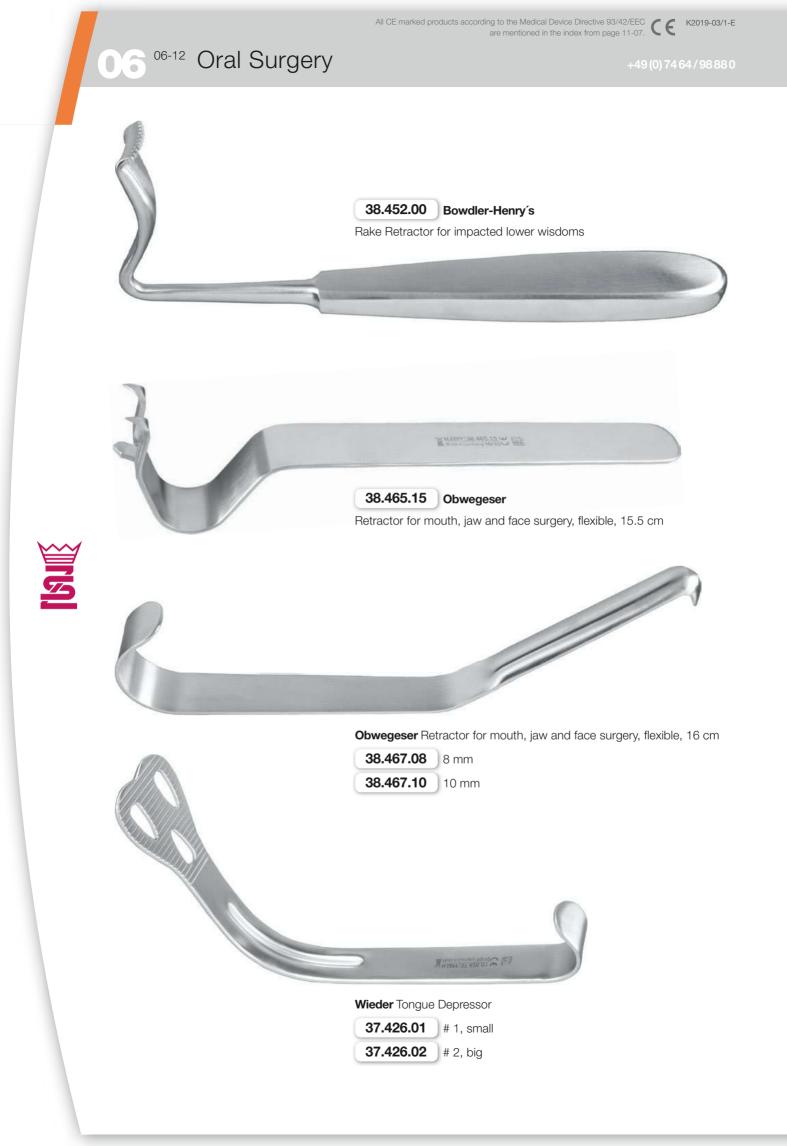




⁰⁶⁻¹⁴ Oral Surgery

+49 (0) 74 64 / 98 88 0

Kocher-Langenbeck

Retractor, 21.5 cm

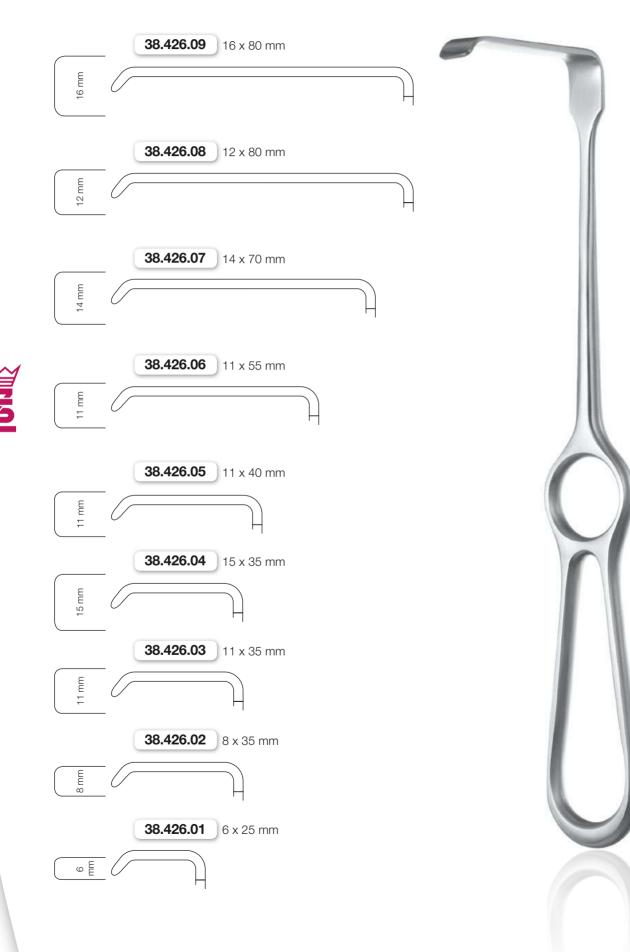


CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E Oral Surgery 06-15 • Combined Retractor and Cheek Retractor Langenbeck by Schäfer Retractor, 21 cm 1 instrument - 2 functions! The combined retractor is suited for an optimized retraction of laps and the cheek during surgery like implantations and root-tip resections. Schäfer Retractor and Cheek Retractor 37.440.00 23 cm 38.430.06 13 x 42 mm 13 mm 38.430.05 11 x 50 mm 11 mm 38.430.04 11 x 40 mm

38.430.04 11 x 40 n

16 mm

38.430.03 16 x 30 mm

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.



0

+49 (0) 74 64 / 98 88 0





06-18 Oral Surgery

+49(0)7464/98880

Laster Special Retractor

Special retractor for upper impacted wisdom teeth

The shape of the handle allows to retract the cheek and the mucoperiosteum and to hold another instrument in the same hand simultaneously.



37.438.15

Laster special retractor for upper impacted wisdom teeth, sandblasted handle, polished working tip and micro serration, 100 mm

ZEPF Vestibulum Retractor acc. to Kapogianni



The **HELMUT ZEPF** Vestibulum Retractor according to Kapogianni is mainly used for the region of the lateral teeth in the upper jaw.



It is meant for the atraumatic holding of the prepared mucoperiosteal flap which is usually retracted in the area of the crista zygomaticoalveolaris. The crista often develops a distinctive osseous bow which makes it impossible to hold it away with a straight retractor.

This instrument is of great advantage especially during operations like the direct sinus lift, big augmentative interventions or other operations in the area from the cuspid to the rear lateral teeth.

Because of the three-dimensional arrangement of both retracting elements of this Vestibulum Retractor, the mucosa is retracted safely and a trauma due to continuous slipping is excluded. Of course, this retractor can be used for anatomically similar bone structures for safe and atraumatic working.

38.448.50

Vestibulum Retractor by Kapogianni, to retract the prepared mucoperiosteal flap

CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E Oral Surgery 06-19 Williger Raspatories Elevators sharp






zepf-dental.com

Oral Surgery 06-21

ZEPF - Raspatories

Perfectly done.

HELMUT ZEPF Periosteal Elevators have a well-balanced design. The lame-design handles have a very handy shape. They are extremely easy to rotate, and due to the smooth surface, hygiene problems known from conventional handles are avoided.

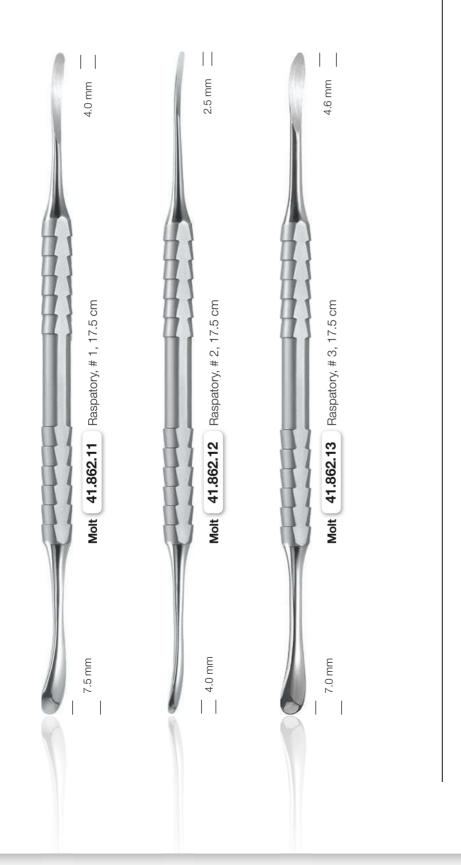



⁰⁶⁻²² Oral Surgery

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0

Prichard

An arrester and raspatory, all in one.

Usable in all types of periodontic surgery, osteotomy, or root-tip resections. Its sharp, rounded tip is used for preparing papilla/loose tissue for excision. In periodontic treatments, its blunt tip allows arresting several flaps of loose tissue simultaneously. The curvature of its blunt tip makes it also a popular choice for osteotomies in the molar area (8-area), as well as for mirror raspas, since its contacting surfaces are highly polished. Lingual surfaces may be very easily reached.



All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E CE

Oral Surgery 06-23

•


Glickmann

Periosteal Elevator and Flap Knife in one instrument.

The flap knife is as sharp as a scalpel. (It has to be resharpened regularly!). Small additional cuts can be made in the interdental area. You do not have to switch to a standard scalpel. The delicate, round and sharp working tip is used to peel off / to cut the flap.

Combination-Instruments

Spiculum Raspatory and round Periosteal Elevator, 17.5 cm

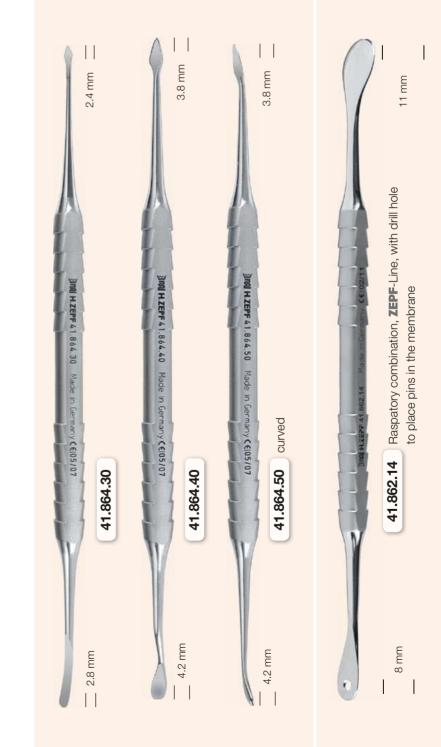





⁰⁶⁻²⁴ Oral Surgery


+49 (0) 74 64 / 98 88 0

Bone Rongeur Forceps Micro Friedmann Micro Bone Rongeur Forceps 2.5 mm 2.0 mm 90°, 14.5 cm 30°, 15.5 cm 30° $^{\circ}06$ 45° 42.362.15 42.358.15 42.360.15 42.315.16 42.316.15 **Micro Friedmann** Blumenthal Bone Rongeur Forceps Bone Rongeur Forceps, 15.5 cm 2.0 mm Q.A # 7 # 42.328.15 42.326.15 42.324.15 42.315.16S Micro Friedmann with La Grange Bending (s-shape) Luer 30°, 15.5 cm Bone Rongeur Forceps, 15 cm

Oral Surgery 06-25

•

Bone Rongeur Forceps

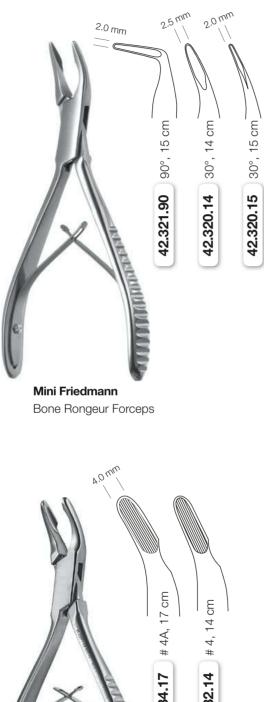



Beyer 18 cm Bone Rongeur Forceps, double action







Zaufal-Jansen 18 cm Bone Rongeur Forceps, double action

6 ⁰⁶⁻²⁶ Oral Surgery

+49 (0) 74 64 / 98 88 0

Bone Cutting Forceps





Ruskin-Liston 18.5 cm Bone Cutting Forceps, double action

curved

42.621.18



zepf-dental.com

Oral Surgery 06-27

•







Controlled dropping of the blade

ZEPF Blade Holder ■Drop-Control>

The **ZEPF** Drop-Control[®] Blade Holder combines the design of the regular blade holder 46.007.00 with a new and revolutionary function. With reference to the mechanism of a ball pen, the blade will be dropped off by pushing the button at the end.


The object of this development was a simplified application with the same diameter of the blade holder. Therefore there is no need to adapt to a new application / ergonomics for our regular blade holder! The **ZEPF** 'Drop-Control[®]' Blade Holder perfectly fits into our **ZEPF** Design product range for surgery, implantology and microsurgery thanks to its diameter, design and ergonomics.

By pressing the button at the end of the blade holder the mechanism which lifts the blade is triggered off. The blade is pushed forward so that it falls safely and controlled in a tray or cup.

Afterwards the one-hand ejection function moves back in its initial position. After cleaning and sterilization you can insert a new blade – as usual.

The advantage lies in the fact that the used blade can be removed in a safe and controllable way in order to prevent a contaminated injury or infection.

Drop-Control

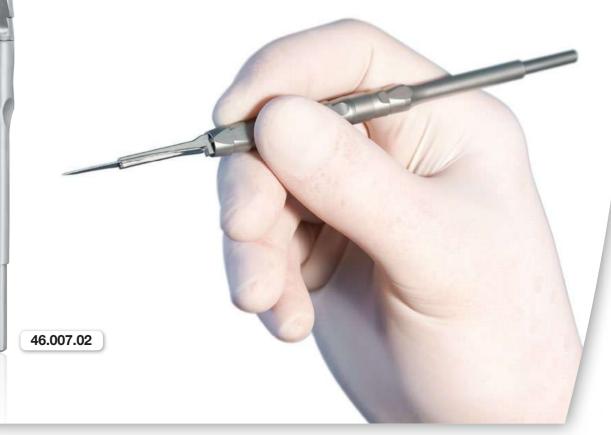

06-28 Oral Surgery

+49 (0) 74 64 / 98 88 0

Scalpel Blades

Supplied in packs of 100 pieces, sterile





Place the blade remover




Press the blade remover



Lever the blade upwards



Pull the blade forward and throw it in a containment

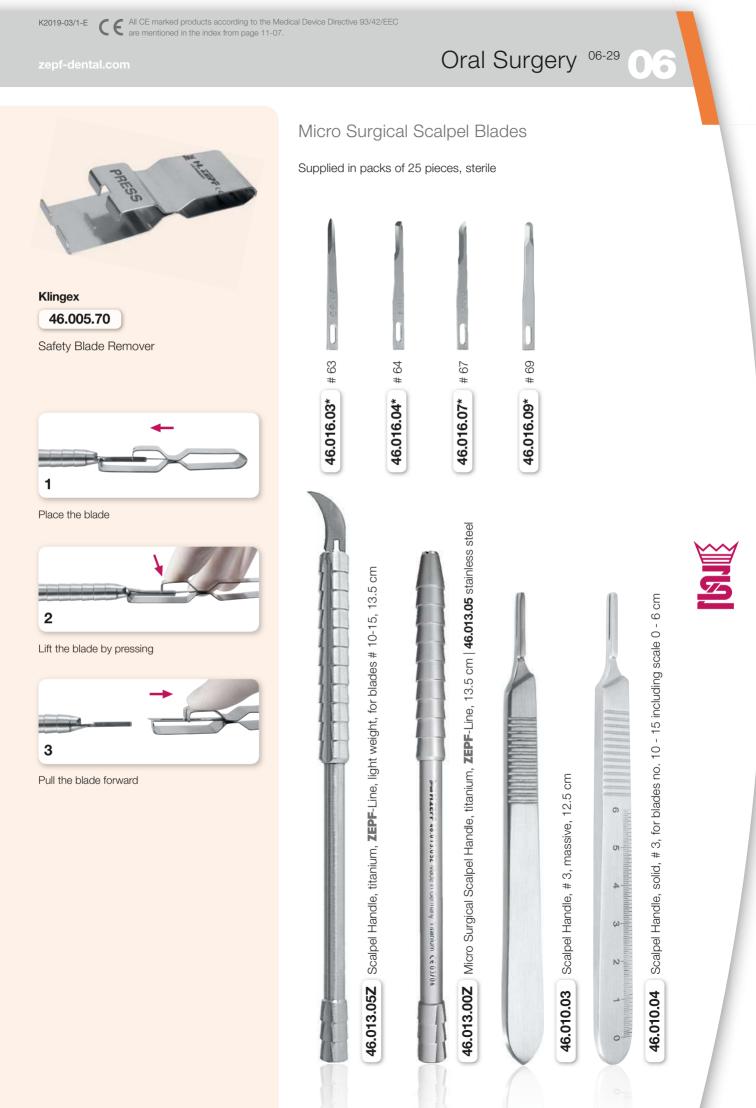

06-30 Oral Surgery

+49 (0) 74 64 / 98 88 0



zepf-dental.com

Oral Surgery 06-31

•


ZEPF Onyx Scissors

The Onyx coating offers a 3-5 times higher surface hardness compared to traditional scissors. In combination with the "Supercut" grinding (see page 06-32), this guarantees an extremely long product life and application with very high precision and wear resistance.

The extraordinary surface smoothness is leading to an easy slide of the scissor blades even under highest strain. Due to the physical / chemical combination of the coating, no undesirable reaction will be caused during sterilization or usage of solvents. Furthermore, the anti-glare surface avoids disturbing light reflections.

The article numbers are complemented by **TISC**. For further information on the illustrated scissors, please refer to the following pages.

46.201.13TISC



46.081.16TISC

Englanding in inter

46.431.14TISC

46.057.11TISC

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁶⁻³² Oral Surgery


+49 (0) 74 64 / 98 88 0



SC stands for "Supercut" and means that scissors with that designation have been specially ground, not only to make them sharper than ordinary scissors, but to yield a much better cutting angle (cf. the accompanying illustrations). One ring is golden.



TC stands for "Tungsten Carbide", a material whose superior strength wear resistance and hardness are its major properties that distinguish it from conventional materials. Both rings are golden.





All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E F C

Oral Surgery 06-33

Fine Preparation Scissors

The curved blunt Preparation Scissors are used for preparation in the least traumatic way of separating tissue into connective tissue layers.

The surgeon pushes the scissor parallel to the skin or to the level of the layers which should be separated (picture 2), opens the scissor and pulls it back in an opened position.

The tissue layers are separated by spreading movements of the scissor blades and the required layer is opened (picture 3). The tip of the scissor is usually facing the less sensitive structures.

In the second instance the scissor is used for cutting.








46.069.11 **Fine Preparation**

Scissors curved, 11.5 cm

Goldman-Fox curved, 13 cm



curved: straight:



serrated edge

46.201.13TC 46.200.13TC 46.200.13TISC



serrated edge

Goldman-Fox compound curved, 13 cm 46.207.13 46.207.13SC

serrated edge

⁰⁶⁻³⁴ Oral Surgery

+49 (0) 74 64 / 98 88 0









All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

06-38 Oral Surgery

+49 (0) 74 64 / 98 88 0

Needle Holder

Swedish Model





06-40 Oral Surgery

+49 (0) 74 64 / 98 88 0

Surgical Aspirators

Curved, with slot against sucking in, 17.5 cm





All CE marked products according to the Medical Device Directive 93/42/EEC ce are mentioned in the index from page 11-07. K2019-03/1-E 06-42 Oral Surgery Retraction-Thread Plugger The ergonomic shape of the instrument tips allows plugging of the thread even in difficult spots. The notch at the tips make it substantially easier to tie the thread around the tooth, the thread remains in the pocket and does not stick to the instrument. The plugger is made of stainless steel and has the new **ZEPF GOOK** Handle. 24.548.01 Retraction-Thread Plugger, exchangeable Probes Antrum Probe


19.576.13	Ø 1.5 mm, 13 cm
19.574.14	Ø 1.0 mm, 14.5 cm
19.576.14	Ø 1.5 mm, 14.5 cm
19.574.16	Ø 1.0 mm, 16 cm
19.576.16	Ø 2.0 mm, 16 cm

Luniatschek

 19.600.18
 Cotton Plugger, 1.8 mm, fine, 17.5 cm

 19.600.25
 Cotton Plugger, 2.5 mm, wide, 17.5 cm





+49 (0) 74 64 / 98 88 0

Wire Seizing / Ligature Pliers and Fracture Splint



zepf-dental.com

Mirrors for Interoral Photography

Titanium-coated front surface for very clear picture.



016

06-46 Oral Surgery

+49 (0) 74 64 / 98 88 0

ZEPF Bone Holding Forceps

acc. to Dr. Howard Gluckman







23.105.50

ZEPF Bone Holding Forceps acc. to Dr. Howard Gluckman



Dr. Howard Gluckman

Specialist in Periodontics, Implantology and Oral Medicine Director of Implant & Aesthetic Academy, Cape Town, South Africa

"Bone holding forceps that I have tried so far are always very difficult to handle and some require 2 hands to use them effectively. A big problem for me was that the forceps usually got in the way and made screwing the bone blocks into position difficult. This inspired me to create a bone holding forceps that allowed one to effectively hold the bone plate or the bone block and at the same time having adequate space for the bone screws and driver.

The holder is easy to use with one hand due to the ratchet design and firmly grips either the bone plate or block on its own, thereby allowing fixation of the plate at the desired distance from the bone; if you utilise the Khoury technique; or to hold both bone block and recipient site thereby enabling easy bone fixation. The bone vice is designed to work with both large and small blocks."








Hammer, Ferrozell

The big hammer lies perfectly in the hand. Due to its (woodlike) material consistency, it offers a superior feeling in osteotomizing. No feel of metal, no loosening of plastic inserts – You always have the feeling of hitting perfectly and of regulating the pressure and the speed...

A true miracle of dental surgery and a must for each OT Set - not only for "big" surgeons!



The instruments illustrated in this catalogue are subject to modifications regarding technical progress and improvements.

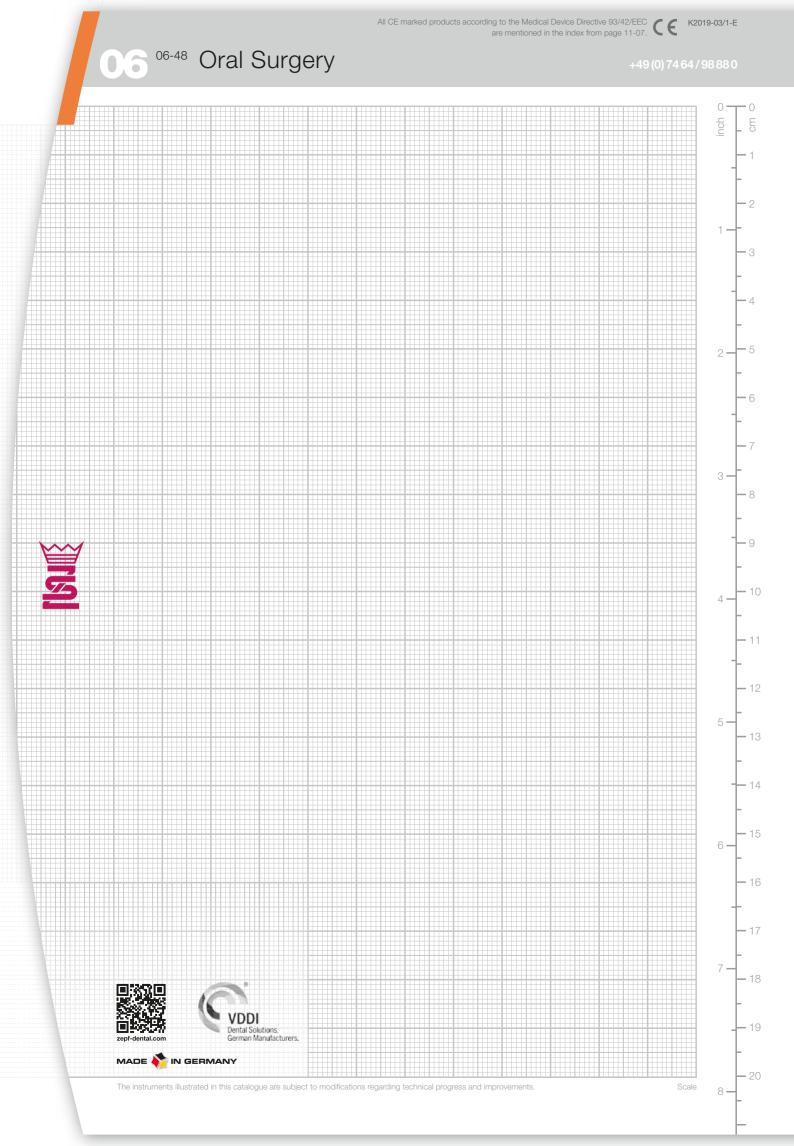



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-02 Implantology

S

+49 (0) 74 64 / 98 88 0

Content: **ZEPF** ECO ImplaTool Set


The ZEPF ECO ImplaTool Set in cobalt-blue


24.961.05 or lightred-magenta

24.961.06

Out of his own experience Dr. Hildebrand came up with a complete instrument set for the whole oral surgery and the treatment in the implantology and periodontalogy. No matter if classical or new conceptions, like sinus elevation or microsurgical interventions, all demands can be covered. Special raspatories, elevators and dissecting instruments enable and simplify surgical procedures and mainly non-traumatic operations.

Clearly organized in a washbasket - so everything is always easily at hand for the practitioner.

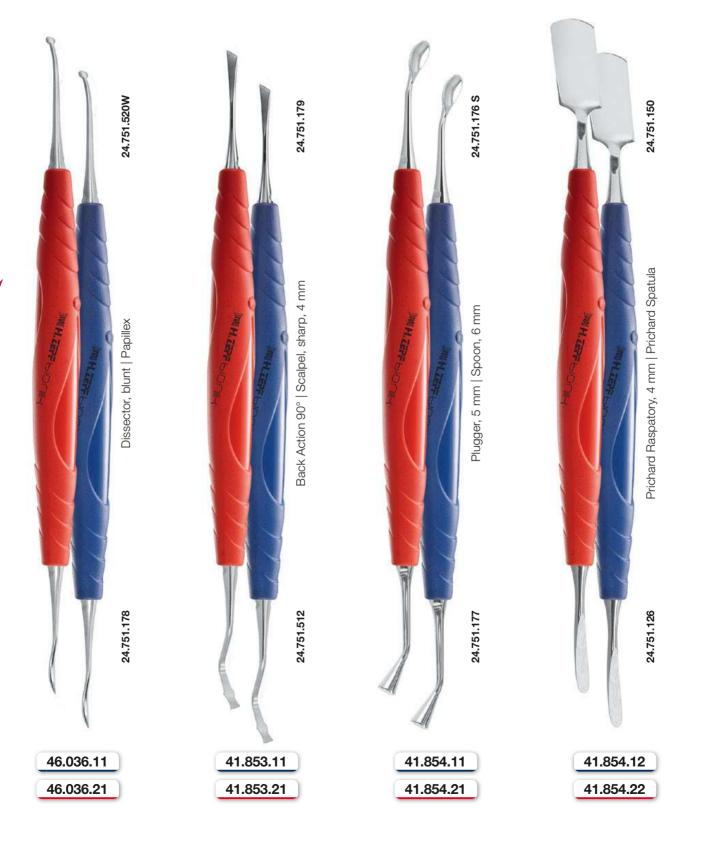

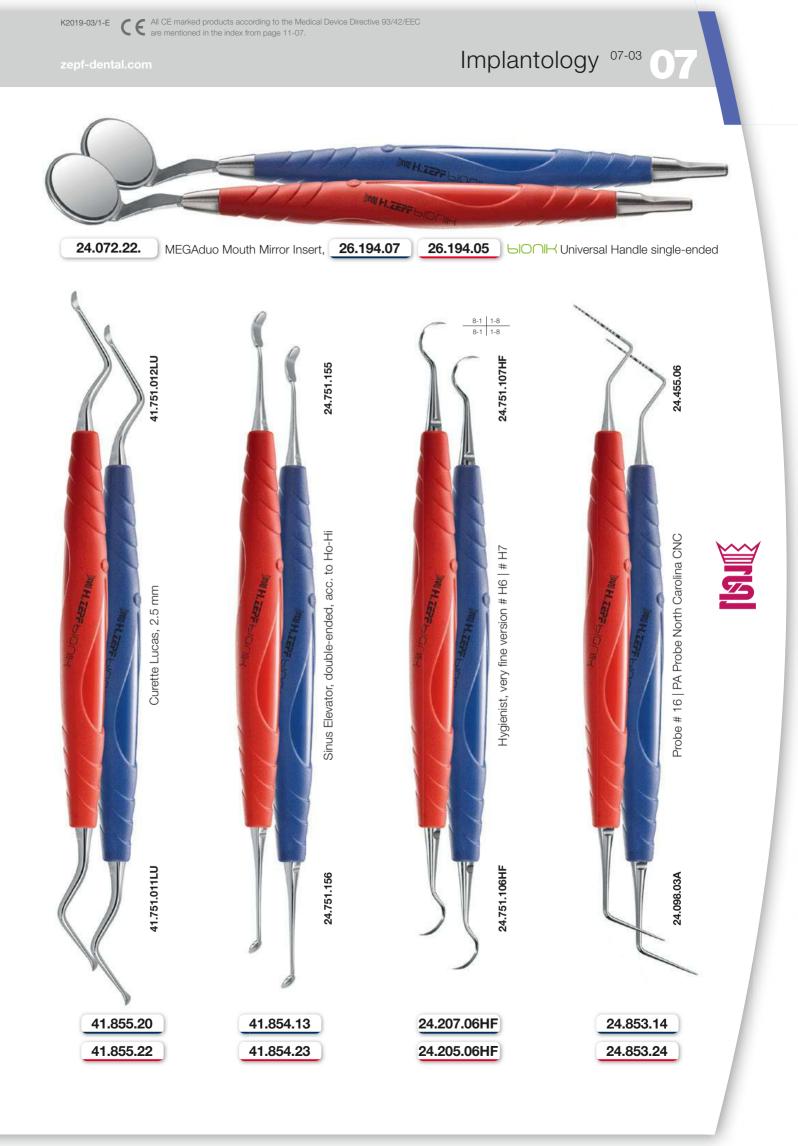

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-04 Implantology

+49 (0) 74 64 / 98 88 0





zepf-dental.com

Implantology 07-05

Bone Scraper

Collecting autologous bone material.

In oral surgery bone replacements and bone structures are often combined with autologous bone pieces during augmentations in order to use their osteoinductive effect. The Bone Scraper is the perfect instrument for an easy and quick collection of autologous bone structures. It enables you to scrape, collect and transplant the patients' own bone. Everything can be done without the usage of bone filter, trephine bur, saw or bone mill.

The blade makes a collection of cortical and spongious bone possible. The bone is collected in a chamber during the scraping and at the same time the bone is being mixed with blood. The bone material can be implanted directly out of the Bone Scraper which has been sterilized before.




ZEPF Bone Scraper II



By using the Bone Scraper, instruments like bone filters, trephines, saws and bone mills are no longer necessary. Its blades allow a fast harvesting of cortical and cancellous bone. The cost-efficient disposable blade offers the practitioner an always sharp and economical instrument.

Spare Blade replacements, available in quantities of: 47.957.30 3 pieces 47.957.50 5 pieces Sleeve 47.957.70 Bone Scraper II **ZEPF**-Design, with sleeve and disposable blade 47.957.10 straight version 47.957.15 angled version **Bone Scraper II Handle** 47.957.60 straight version 47.957.65 angled version **Essential advantages:** ergonomic easy cleaning quickly replaceable blade simple application



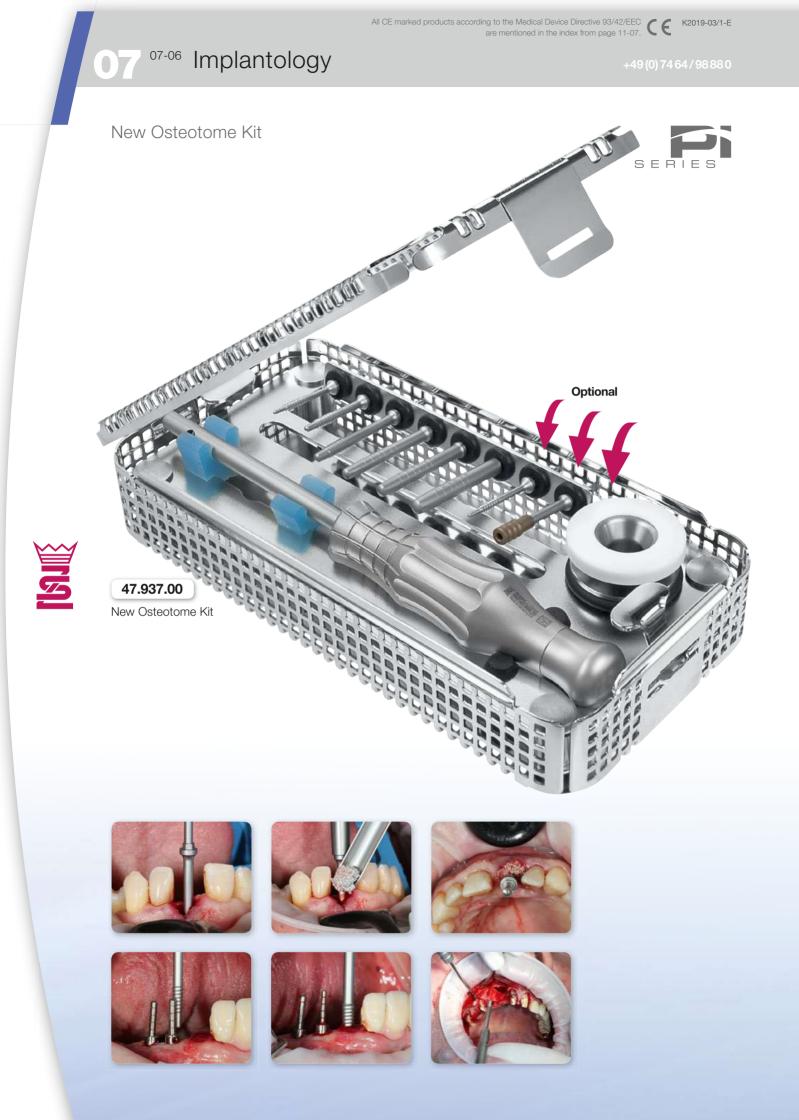





47.937.10 Ø shank 2.7 mm, Ø tip 2.0 mm

New Osteotome Inserts RA-Hex connection with shock absorption, graduation 7/10/13/15/18/20 mm



47.502.10

Screwdriver Handle with extension, RA-Hex connection with shock absorption, for screwing and hammering application

Without illustration

85.182.50	1/3 Washtray System
47.937.01	Tray for New Osteotome Kit

Optional Accessories




47.950.03

Pin Applicator, short, to apply titanium pins

85.255.02

Storage Box for 10 titanium pins

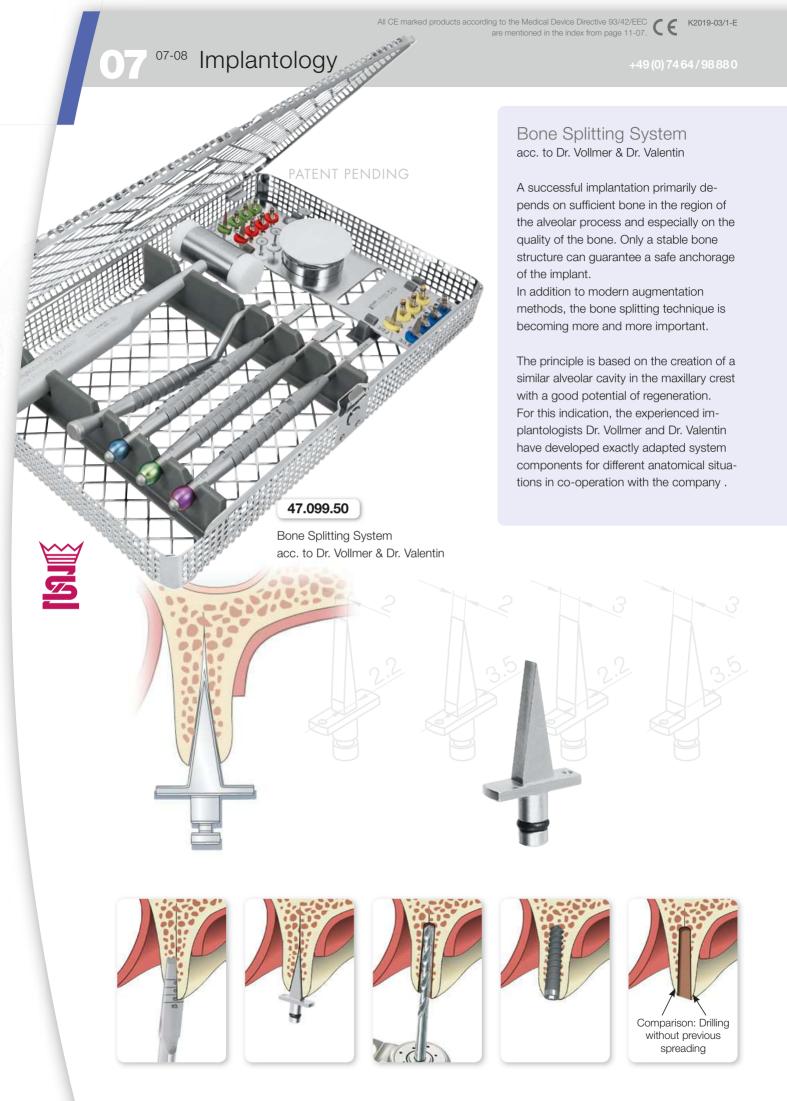


zepf-dental.com

Implantology 07-09

At first, the maxillary crest which has become too small due to atrophy is being separated in its longitudinal direction by diamond discs. Thereafter, it is split carefully by means of chisels. In doing so, the lateral cortical bone lamellae are preferably displaced in labial direction.




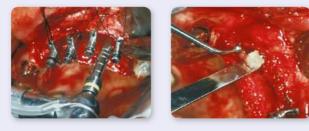

After these preparatory steps, small wedges are inserted in the gap. In each case, two wedges are used as placeholders for the drilling of the implant bed and the insertion of the implant.

While drilling, the bone lamellae are reliably prevented from springing back. Upon insertion of the implants and removal of the inter-implantatory wedges, the remaining gaps can be filled with augmentation material in order to allow an augmentation and, in opportune cases, an immediate and simultaneous implantation.



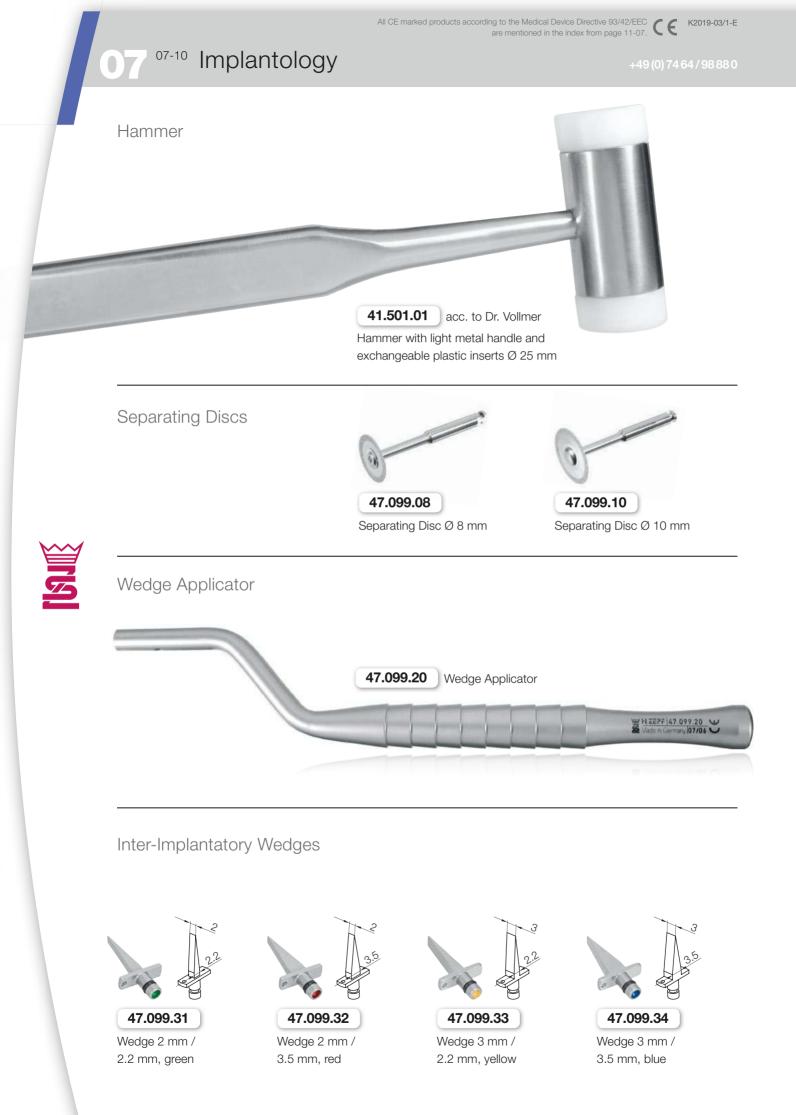


zepf-dental.com

Implantology 07-11

Back Action Chisel

Modified as Bone Scraper in different widths, to gain autologous bone during operation.

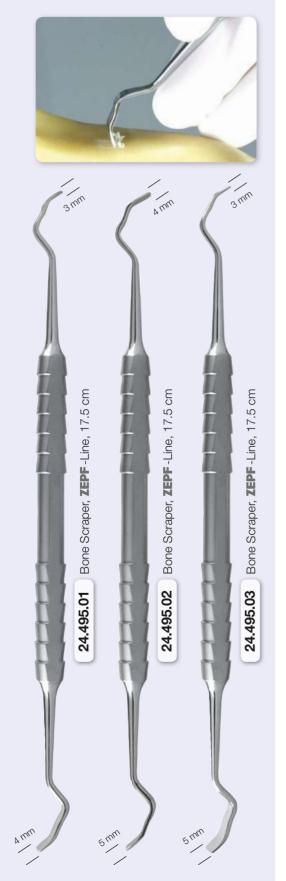


Bone Fitting Set acc. to Dr. Hohl & Dr. Hildebrand



Bone chisels are used to gain bone chips, to shape bone structures and to widen bones from the cranial side. The pointed chisels are used for the first widening of the maxillary crest. The flat chisels smoothen and shape bone structures.




Content: Bone Fitting Set



flat	
47.949.21	(4.0 mm)
47.949.22	(6.0 mm)
47.949.23	(8.0 mm)



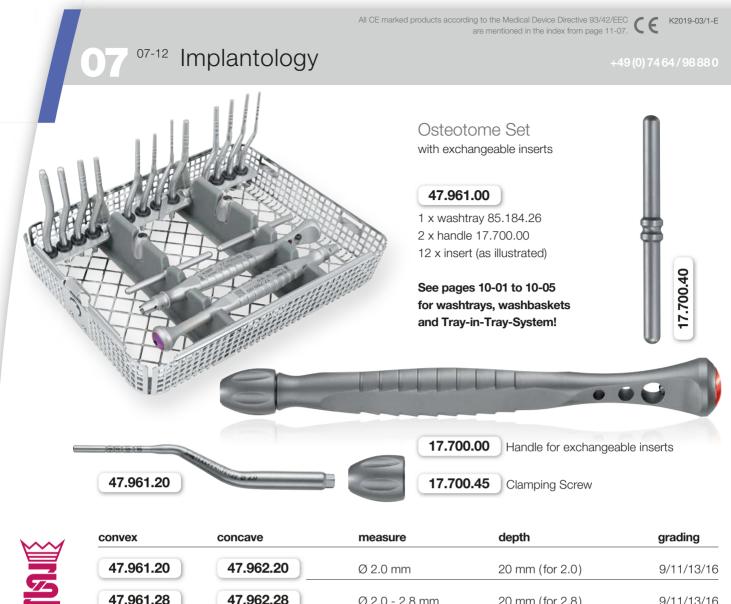

47.301.20	47.302.20	0 2.0 - 2.8 11111	20 11111 (101 2.8)	9/11/13/10
47.961.33	47.962.33	Ø 2.8 - 3.3 mm	20 mm (for 3.3 / 3.8)	9/11/13/16
47.961.38	47.962.38	Ø 3.4 - 3.8 mm	20 mm (for 4.3)	9/11/13/16
47.961.43	47.962.43	Ø 3.9 - 4.3 mm	20 mm (for 5.0 / 6.0)	9/11/13/16
47.963.50	47.962.50	Ø 5.0 mm	20 mm (for 5.0)	-
47.963.60		Ø 6.0 mm	20 mm (for 6.0)	-

Hollow Cylinder Osteotomes acc. to Dr. Vollmer & Dr. Valentin

With the ejector, which will positioned at the distal end, the gained bone material can be implanted efficiently in another place. Comparable with solid osteotomes it comes to a condensing of the bone in order to get a better primary stability for the implant in a cancellous bone.





zepf-dental.com

Implantology 07-13

Osteotome Set



Osteotome Set, straight

47.940.01

Osteotome Set, angulated

always including

85.180.00

Washtray 1/1, for max. 16 hand instruments incl. 2 silicone rubbers and instrument retainer, 275 x 178 x 24 mm




47.945.38

47.945.43

Ø 3.4 / 3.8 (for 4.3)

Ø 3.9 / 4.3 (for 5.0 / 6.0)



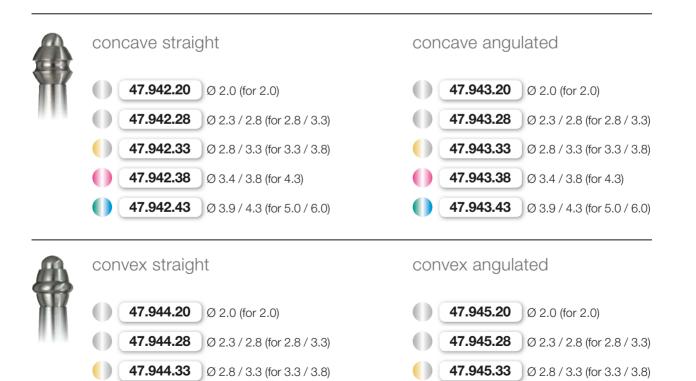

47.944.38 Ø 3.4 / 3.8 (for 4.3) **47.944.43** Ø 3.9 / 4.3 (for 5.0 / 6.0)



All CE marked products according to the Medical Device Directive 93/42/EEC ${\rm CE}$ are mentioned in the index from page 11-07. K2019-03/1-E



zepf-dental.com


Implantology 07-15

Advantages of the VGO Osteotomes

- ZERO HEAT PRODUCED!
- ALWAYS PASSIVE ENTRANCE!
- DECREASED CRESTAL STRESS!
- FULL CONTROL OF RATE OF DILATION! since hand-piece is not used at constant speed
- REVOLUTIONARY FLEXIBILITY OF USE All Osteotomes on the market may look alike, but they are **not**! We offer a unique stepped formula for tip escalation and a revolutionary flexibility of use like no other system on the market.

3 MAIN MODES OF USE!

ZEPF VGO MODE: **PASSIVE ENGAGEMENT (Stepped Escalation) ZEPF** HYBRID MODE: **PASSIVE ENGAGEMENT (Linear Escalation) ZEPF** STANDARD MODE: **PASSIVE ACTIVE ENGAGEMENT / NON ENGAGEMENT** not recommended

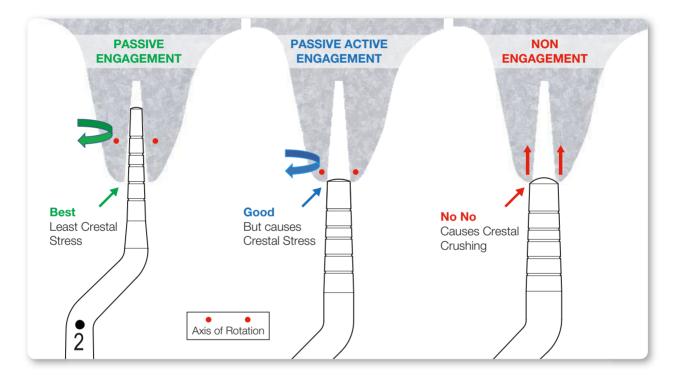

Bone is Gold: PASSIVE WAVE DILATION SYSTEM acc. to Pavel Krastev DDS

How do we manage the osteotomy ATRAUMATICALLY? How do we manage the osteotomy for greater implant success? Bone is Gold, so how do we hurt the bone less? How do we mallet less, as to make procedure less unpleasant for our patients?


Let us control the bone as opposed to having the bone control us.

Because of the overlapping diameters of the **VGO** Osteotomes, you are able to passively engage the previously made intrabony cavity, even when you didn't use the full length of the tip. **PASSIVE ENGAGEMENT** – successive osteotome fits freely into the previous intrabony cavity and becomes active at a point deeper than crestal bone, as is currently done by the new **ZEPF VGO** Way.

PASSIVE ACTIVE ENGAGEMENT – when a traditional Summers Osteotome is used to full working depth of tool, the next tip will engage previously made intrabony cavity passively and will start being active immediately as it progresses further into cavity.

NON ENGAGEMENT – when next osteotome is used, it simply does NOT fit the intrabony cavity created by previous osteotome. This is what occurs when traditional Summers Osteotomes are used to partial depth of tip. All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E (ϵ) are mentioned in the index from page 11-07.

07-16 Implantology



VGO Ost-Set - straight, in a Washbasket with Lid (REF 85.194.22) containing:

Included in both sets:

ANTERIOR VGO OST-Set

with 7 straight screw osteotome inserts, numbered from 0-6


- Tips have first 8 mm threaded
- Produce micro cuts in bone
- Increased bleeding and better angiogenesis
- No malleting needed
- Tip-0 is unique in straight kit (Ø 1 Ø 2 mm)
- Tip-0 to accommodate thin anterior ridges
- Provides precision marking tips for immediate placement

17.710.00 Z-Shape Universal handle & instrument holder for inserts with HEX-adapter, AF4, sandblasted, 2 pieces included in the set 111 300 H ZEPF 47.990.06 Ind H.ZEPF 47.990.08 47.990.06 Precision Marking Tip, bent, 47.990.08 Precision Marking Tip, straight, scale 8/10/13/16 mm scale 8/10/13/16 mm Straight Screw Osteotomes in the VGO OST-Set ·U· 51 INU H.ZEPF 47.990.10 Exchangeable with Hex Connection for Z-Shape Universal handle Ø 2 Ø 1 <u>در</u> ∙⊙• amm 47.990.10 Screw Osteotome Insert straight, size 0, tapered Ø 1 - 2 mm, convex shank Ø 2 mm, <u>Ø 3</u> scale 8/10/13/16 mm Ø 1 S2 47.990.20 ann -Screw Osteotome Insert straight, size 1, tapered Ø 1 - 3 mm, convex shank Ø 3 mm, scale 8/10/13/16 mm ØЗ <u>Ø2</u> 47.990.30 Screw Osteotome Insert straight, size 2, amm • 🔁 လဲ tapered Ø 2 - 3 mm, convex shank Ø 3 mm, Ø 4 scale 8/10/13/16 mm Ø 2 47.990.40 TIIID က္ Screw Osteotome Insert straight, size 3, н tapered Ø 2 - 4 mm, convex shank Ø 4 mm, Ø 4 scale 8/10/13/16 mm ØЗ SIS S IIIII 47.990.50 Screw Osteotome Insert straight, size 4, •4 tapered Ø 3 - 4 mm, convex shank Ø 4 mm, Ø 5 scale 8/10/13/16 mm ØЗ 47.990.60 d M юe н Screw Osteotome Insert straight, size 5, tapered Ø 3 - 5 mm, convex shank Ø 5 mm, <u>Ø5</u> scale 8/10/13/16 mm Ø 4 20 47.990.70 •0 Screw Osteotome Insert straight, size 6, tapered Ø 4 - 5 mm, convex shank Ø 5 mm, scale 8/10/13/16 mm



zepf-dental.com

Implantology 07-17



47.991.00

VGO Ost-Set – angulated, in a Washbasket with Lid (REF 85.194.22) containing:

ØЗ

ØЗ

Ø 4

<u>Ø4</u>

<u>Ø5</u>

Ø 5

<u>Ø 6</u>

Ø 6

Ø 1

Ø 2

ØЗ

ØЗ

Ø 4

Ø 4

<u>Ø5</u>

Cortical bone lines socket Purchase point Osteotomy to follow purchase point 47.990.06 47.990.08

.....

• 🔁

က္

•4

Ω●

• o

▶•

• ∞

POSTERIOR VGO OST-Set

with 8 angulated osteotome inserts, numbered from 1-8

- No threads since turning motion limited
- 5 mm mark placed on all tips to mark threshold for crestal lift
- 5 mm is minimum available bone recommended for crestal lift
- Tips have same taper as tips 1-6 for straight kit
- Two additional tips (7 and 8) to accommodate wider ridges typically found in posterior area
- Provides precision marking tips for immediate placement

Application of the Precision Marking Tips

To be used during immediate placement surgery to initiate osteotomy offset towards palatal. Rotary drills usually slide down bone due to angle at which the osteotomy is initiated.

Angulated Osteotomes in the VGO OST-Set

Exchangeable with Hex Connection for Z-Shape Universal handle

47.991.10	Osteotome Insert angulated, size 1, tapered Ø 1 - 3 mm, convex shank Ø 3 mm, scale 5/8/10/13/16 mm
47.991.20	Osteotome Insert angulated, size 2, tapered Ø 2 - 3 mm, convex shank Ø 3 mm, scale $5/8/10/13/16$ mm
47.991.30	Osteotome Insert angulated, size 3, tapered Ø 2 - 4 mm, convex shank Ø 4 mm, scale 5/8/10/13/16 mm
47.991.40	Osteotome Insert angulated, size 4, tapered Ø 3 - 4 mm, convex shank Ø 4 mm, scale 5/8/10/13/16 mm
47.991.50	Osteotome Insert angulated, size 5, tapered Ø 3 - 5 mm, convex shank Ø 5 mm, scale 5/8/10/13/16 mm
47.991.60	Osteotome Insert angulated, size 6, tapered Ø 4 - 5 mm, convex shank Ø 5 mm, scale 5/8/10/13/16 mm
47.991.70	Osteotome Insert angulated, size 7, tapered Ø 4 - 6 mm, convex shank Ø 6 mm, scale 5/8/10/13/16 mm
47.991.80	Osteotome Insert angulated, size 8, tapered Ø 5 - 6 mm, convex shank Ø 6 mm, scale 5/8/10/13/16 mm



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-18 Implantology

+49 (0) 74 64 / 98 88 0


3D One Step Augmentation & Implantation

acc. to Dr. Bernd Giesenhagen

In co-operation with Dr.Giesenhagen, the company **HELMUT ZEPF** has developed a new set for the One Step Vertical Augmentation with ring-shaped bone transplants.

The aim of this development is an accelerated implant treatment. Thereby, the safety of the implantological success as well as the convincing result for the patient and the user have priority. In many cases, this new augmentation method can be used to build up the bone base for the insertion of one or more implants.

Particularly suitable for the vertical augmentation of the highly atrophied and distal mandible (pic. 2). With this newly introduced technique, perfectly fitting ringshaped bone transplants are removed from the chin-, retro-molar region or from the palatal area (pic. 1) by means of trephines and fixed immediately in the receiving area (pic. 3) with a screw implant.

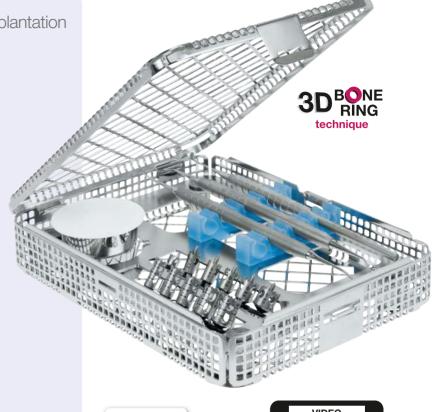

47.500.31

Complete Set with washbasket 85.184.18 and instruments; without optional accessories






Dr. Bernd Giesenhagen, the inventor of this procedure, and **HELMUT ZEPF** have selected a special range of instrumenta-

tion for precise and time-saving steps of treatment in order to ensure an optimal

function.



Application

The local cortical bone structure with spongious parts of vital cells guarantees a safe fixation with short healing time.

The filling of possibly existing cavities is usually made by spongious chips taken from the donor area or by bone substitutes.

For an additional coverage of the augmented area with a barrier membrane we recommend our **HELMUT ZEPF** Augmentation Kit 47.966.00.







07-20 Implantology

+49 (0) 74 64 / 98 88 0

Trephines

Trephines are used for a gentle and precise removal of an implant. They are used to win bone texture and to excavate implants accurately. The trephines are manufactured of stainless steel. The grading is visibly laser-marked onto the burs and guarantees a secure depth orientation.

The windows in the body offer a better view for the excavation of the implants and make it easier to reject fragments. The bur stand offers a safe and perfectly clean storing and easy positioning through a snap-in system.

The marking of the rack allows a fast and uncomplicated identification of the trephines.



Bur Stand for Trephines



for 6 burs, shaft	t Ø 2.35 mm
85.070.05	8.5 x 4.5 cm
for 6 short burs	, shaft Ø 2.35 mm




	Ø Inside	Ø Outside	Teeth	Body Length	Grading
08.910.01	1.7 mm	2.3 mm	7	22 mm	7/10/13/16
08.910.02	2.3 mm	2.8 mm	7	22 mm	7/10/13/16
08.910.03	2.8 mm	3.3 mm	9	22 mm	7/10/13/16
08.910.04	3.3 mm	3.8 mm	9	22 mm	7/10/13/16
08.910.05	4.0 mm	4.5 mm	11	22 mm	7/10/13/16
08.910.06	4.3 mm	4.8 mm	11	22 mm	7/10/13/16
08.910.07	4.8 mm	5.8 mm	9	22 mm	7/10/13/16
08.910.13	5.0 mm	6.0 mm	11	22 mm	7/10/13/16
08.910.08	6.0 mm	7.0 mm	12	22 mm	7/10/13/16
08.910.09	7.0 mm	8.0 mm	18	22 mm	7/10/13/16
08.910.10	8.0 mm	9.0 mm	18	22 mm	7/10/13/16
08.910.11	9.0 mm	10.0 mm	18	22 mm	7/10/13/16
08.910.12	10.0 mm	11.0 mm	19	22 mm	7/10/13/16



	Ø Inside	Shaft	Description
08.911.30	3.0 mm	2.35 x 15 mm	Trephine short
08.912.50	5.0 mm	2.35 x 15 mm	Trephine short
08.912.75	7.5 mm	2.35 x 15 mm	Trephine short
08.912.10	10.0 mm	2.35 x 15 mm	Trephine short

MUCOSA Membrane Punches suitable for hand piece (Dimensions are the inner diameter)

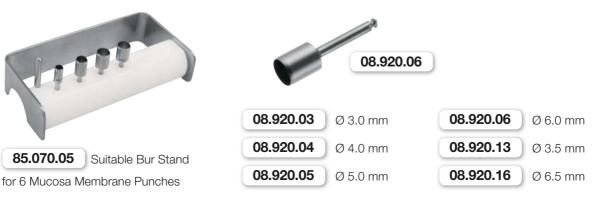

zepf-dental.com

Implantology 07-21

ZEPF Bone Crusher

With this Bone Crusher we introduce a proven alternative to the more complex bone mill. Insert the bone piece into the crusher and use the Pusher in order to crush the bone. If necessary, you may additionally use the hammer 41.509.00.

Bone Mill Forceps

For gaining autogenic bone material.

In order to correct bone defects, an intraoral harvesting of bone is often necessary. Pieces of bone may be gained with trephines or chisels. It is the aim of the Bone Mill Forceps to cut bone material into small pieces so that a maximum volume of bone chips can be achieved. The "grainy" consistency of bone chips created will ensure that it is adapted most favourably to osseous embedding.



07-22 Implantology

+49 (0) 74 64 / 98 88 0



47.954.01

ZEPF Bone Mill, to crush autologous bones, with helically toothed milling part



47.954.35

Helical toothed Milling Part

for Bone Mill 47.954.01 and to be mounted in 47.954.00 / 47.954.01 (This new milling part can be ordered and subsequently be mounted in an older type of Bone Mill by the user himself).

ZEPFbonemill()())

47.954.55

Extension Bar for the rotary handle 47.954.50, to increase the lever effect



ZEPF Bone Mill

Bone Mill, to crush autologous bones. In order to correct bone defects, bone harvesting is necessary elsewhere. Bigger bone pieces or boneblocks can be removed by using trephines.

The **ZEPF** Bone Mill allows to crush bone in order to produce the greatest possible volume of bone graft. The grainy consistence of the produced bone graft guarantees an optimal adaption on the bone.

The extension bar which can be adapted on the rotary handle facilitates an optimized power transmission and torque. The new Bone Mill with helical toothed milling part makes milling easier.

Advantages of the **HELMUT ZEPF** Bone Mill:

- easy handling
- quick assembly / disassembly without additional tools
- no loss of bone material (even in the case of small quantities)
- easy cleaning

zepf-dental.com

Implantology 07-23

Sinus Elevators acc. to Dr. Meiselbach

The 3 Sinus Elevators acc. to Dr. Meiselbach enable a gentle and atraumatic sinus floor elevation in all areas.

Due to their special shaping the Elevators are an ideal addition to the Universal Sinus Instruments.





07-24 Implantology

+49 (0) 74 64 / 98 88 0

Universal Sinus Instruments

For implantological treatment in the maxilla, in case of missing vertical bone in the direction of sinus maxillaris.

Advantages:

- angled instruments ergonomically and anatomically optimised
- atraumatic preparation and lifting of the sinus mucosa
- effective working due to a wide range of different angles



zepf-dental.com

Microsurgical Sinus Lift Instruments

Implantology 07-25

For microscopically guided elevation of the sinus bottom acc. to Dr. Behnam Shakibaie-M.

41.847.00

Sinus Lift Instrument Set for microscopically guided elevation of the sinus bottom acc. to Dr. Shakibaie-M. incl. 1 x washbasket 85.195.00 and instruments illustrated on page 07-16 /17







For the development of the new microsurgical sinus lift instruments acc. to Dr. Shakibaie-M., we resorted to the approved conventional shapes of sinus lift instruments.

The new instruments are approx. 60% smaller, they were sharpened and the surface was abraded. Under appropriate optical magnification and illumination of the operation field (operation microscope or magnifying glass), those features offer the following essential advantages:

- The reduction of the instrument size allows the preparation of a minimalized antral window without restricting the qualities of elevation or augmentation.
- The sharpening of the instruments allows a precise initial fracture of the bone layer which is as thin as parchment. The initial fracture is possible as soon as the window is prepared by rotating the instrument, without injuring the Schneider's membrane.
- The delicate coarseness of the surface of the instruments prevents the unpleasant reflection of light from the operating microscope or the magnifying glass.

In addition, the working tips of the instruments were bent in accordance with the reduced sinus lift window.

Finally, the instruments were also numbered and colorcoded to allow an easy, chronological use.

Thus, the surgeon is able to increase the safety during elevation of the sinus bottom and to apply this technique in a minimally invasive way for the patient.

Pictures by Dr. Behnam Shakibaie-M.



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-26 Implantology

97

Microsurgical Sinus Lift Instruments acc. to Dr. Shakibaie-M.

		41.847.00	
		Sinus Lift Instrument Set for microscopically guided elevation of the sinus bottom double-ended, acc. to Dr. Shakibaie-M. contains following components:	
		Jul H. ZEPF 41.847.08 Made in Germany C€107/07 by Dr. Shakibaie-M.	
		41.847.08 Sinus Lift Instrument # 1, sharp, 2.9 / 2.4 mm, green	
		Junil H. ZEPF 41.847.01 Made in Germany CE107/07 by Dr. Shakibaie-M.	
		41.847.01 Sinus Lift Instrument # 2, sharp, 2.9 / 2.9 mm, black	
		■MIH.ZEPF 41.847.05 Made in Germany C€107/07 by Dr. Shakibaie-M.	
1		41.847.05 Sinus Lift Instrument # 3, sharp, 2.8 / 2.9 mm, 45° curved, blue	
		Ingl H. ZEPF 41.847.02 Made in Germany C€107/07 by Dr. Shakibaie-M.	
		41.847.02 Sinus Lift Instrument # 4, sharp, 2.8 / 3.8 mm, white	
		Sng H.Z. PF 41.847.03 Made in Germany C€107/07 by Dr. Shakibaie-M.	
		41.847.03 Sinus Lift Instrument # 5, sharp, 3.6 / 4.2 mm, orange	
		DMILH.ZEPF 41.847.10 Made in Germany CE107/07 by Dr. Shakibaie-M.	
		41.847.10 Sinus Lift Instrument # 6, sharp, 2.3 / 2.3 mm, red	
		JMI H.ZEPF 41.847.09 Made in Germany C€107/07 by Dr. Shakibaie-M.	
	(41.847.09 Sinus Lift Instrument # 7, sharp, 2.1 / 2.1 mm, yellow	

All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E CE

Implantology 07-27

08.906.014C

Diamond, 014C, round, Ø 1.4 mm

08.906.016C

Diamond, 016C, round, Ø 1.6 mm

08.906.018C

Diamond, 018C, round, Ø 1.8 mm



41.868.09 Micro Sinus Spoon, Spoon Ø 8×10 / Ø 4×6 mm, titanium handle, blue,

acc. to Dr. Shakibaie-M.

double-ended, 17.5 cm,

85.251.03

Mixing Cup, stainless steel, with plastic lid, Ø 40 mm, 2 pieces included in the set





19.651.15M Micro Sinus Aspirator

ZEPF 19.651.15M Nade

any CE 105/0

Sinus-Line, titanium tip modified acc. to Dr. Shakibaie-M. All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-28 Implantology

+49 (0) 74 64 / 98 88 0







24.995.01

Complete Set incl. 1 x washbasket with lid 85.195.00 and partition for Sinus Instrument Set acc. to **Prof. Dr. Dr. Stiller**



Sinus Instrument Set acc. to Prof. Dr. Dr. Stiller

Immediate sinus floor elevation with or without bone cover

The Sinus Instrument Set has been developed together with Prof. Dr. Dr. Stiller and is particulary suited for difficult maxillary sinus structure (septa, maxillary pillars, scarred mutations in change with intact maxillary sinus mucosa).



Advantages of the system:

- Instruments which are adapted and adjusted perfectly to the anatomical conditions in the maxillary sinus.
- Flexible working ends. Instruments are pre-bended for the normal enantral anatomy.
- Two different kinds of instruments with blunt and sharp edges for dissecting mucosa on plane and rough internal surface of the maxillary sinus.





All CE marked products according to the Medical Device Directive 93/42/EEC **K2019-03/1-E** are mentioned in the index from page 11-07.

07-30 Implantology

+49 (0) 74 64 / 98 88 0



Sinus Instrument Set acc. to Dr. Kirsch

24.995.00

Complete Set incl. 1 x washbasket with lid 85.195.00 and arrangement for Sinus Instrument Set acc. to **Dr. Kirsch**

Washtrays and washbaskets, Tray-in-Tray-System, see pages 10-01 to 10-05!





⁰⁷⁻³² Implantology

-49 (0) 74 64 / 98 88 0

47.966.00 Augmentation Kit

Augmentation Kit



Reasons for reconstruction of alveolar ridge arise out of defects in the jaw ridge areas. The most frequent causes are: Atrophy of the alveolar ridge and extraction defects.

Out of esthetic reasons alone, in visible areas, these defects need to be reconstructed.

The augmentation is carried out with autologous bone and titanium foil. The bone implants are covered with a titanium foil after application. To avoid dislocation of the augmentation material below the membrane, the membrane is fixed with at least 2 pins.

The titanium pins with 3 mm or 5 mm length are taken out of the storage box by means of the applicators and pressed into the bone through the foil or membrane.



85.255.02

Storage Box for

10 titanium pins,

optional

zepf-dental.com

Implantology 07-33

ustration	Article Description	Order Quantity
	47.966.00 Augmentation Kit, consisting of: Pin Membrane Probe, Pin Applicator, Perforation Raspatory, Sinus 7 Instrument, Titanium Pin 3 mm (10 pieces) / 5 mm (5 pieces), Sinus Elevator # 2, Mixing Cup, Storage Box, 1/2 Washbasket with Lid 85.194.15	1 set
	47.520.00 Pin Membrane Probe with ZEPF -Design handle	1 piece
All and a second se	 47.520.01 Pin Applicator 	1 piece
	47.520.02	1 piece
	Perforation Raspatory 47.520.03 Sinus 7 Instrument acc. to Kirsch, Spoon Ø 6.0 mm / flexible Plugger Ø 5.0 mm	1 piece
~	47.560.03 Titanium Pin, 3 mm (10 pieces included in the set)	5 pieces
_	47.560.05 Titanium Pin, 5 mm (5 pieces included in the set)	5 pieces
	47.847.11 Sinus Elevator # 2, single-ended, flexible	1 piece
	85.251.04 Mixing Cup, stainless steel, with plastic lid, Ø 4 cm	1 piece
Alternative and a second	85.256.00 Storage Box, for 5 soft tissue pins and 10 titanium pins	1 piece
	85.255.02 OPTION Storage Box for 10 titanium pins, optional, if a compact solution is requested	1 piece

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-34 Implantology

+49(0)7464/98880




ZEPF Augmentation Material Applicator

The Augmentation Material Applicator supports the fractional filling of the subantral area with particulate augmentation material. To compact the augmentation material you use a sinus plugger.

The instrument with diameter of 5 mm is loaded laterally.

The augmentation material can be applicated precisely with the injecting mechanism. The instrument can be taken apart for optimal cleaning.



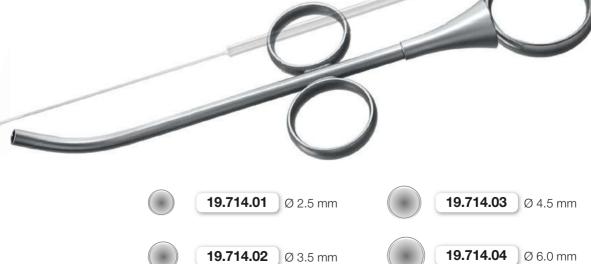

zepf-dental.com

Implantology 07-35

Drilling Sleeves acc. to Prof. Dr. Yildirim






outer Ø: 3.0 mm; inner Ø: 2.05 mm; length: 10 mm (10 pieces)

08.915.02

outer Ø: 3.5 mm; inner Ø: 2.55 mm; length: 10 mm (10 pieces)

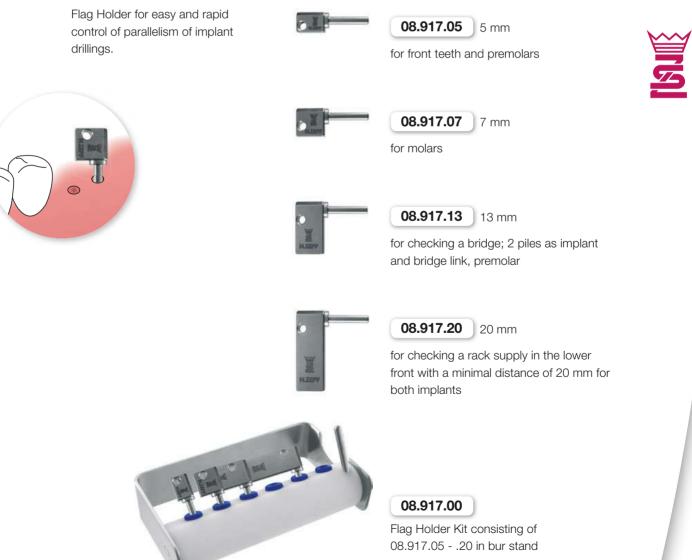

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-36 Implantology

+49 (0) 74 64 / 98 88 0



Krekeler Sliding Caliper

Acc. to Prof. Dr. med. dent. Gisbert **Krekeler** Modif. Dr. med. dent. Sven Marcus Beschnidt

The Sliding Caliper combines a variety of functions in one instrument, thus facilitating the positioning of implants and enlarging the precision.

The measuring rods have a thickness of exactly 1.5 mm and allow immediate control of the maximum diameter of the implant which has to be inserted. (In order to assure maximum stability, please chose the largest diameter). Scientific examinations proved that the wall of the bone should have a thickness of at least 1.5 mm in order to avoid bone resorption after implantation. If the sliding caliper with its two measuring rods is inserted in the interproximal gap and opened in such a way that the measuring rods touch the respective root of the neighbor teeth, the maximum possible diameter of the future implant is shown on the marking IN. The upper marking OUT shows the determined outside dimension.

The new locating screw, at the end of the caliper, allows a fixation of the measured result. This practice-oriented development represents a significant relief with regard to a **more precise, quick and and secure work**.



OUT shows the determined outside dimension (Ø 1.5 mm), **IN** shows the inner diameter.



Locating screw for a safe fixation of the measured result.



The hole serves as drilling gauge and drilling guide. The marking allows the determination of the ridge.




31.693.10

Sliding Caliper acc. to Prof. Dr. med. dent. Gisbert **Krekeler** for measuring of implants with locating screw

zepf-dental.com

Implantology 07-37

Sliding Calipers and Metal Ruler

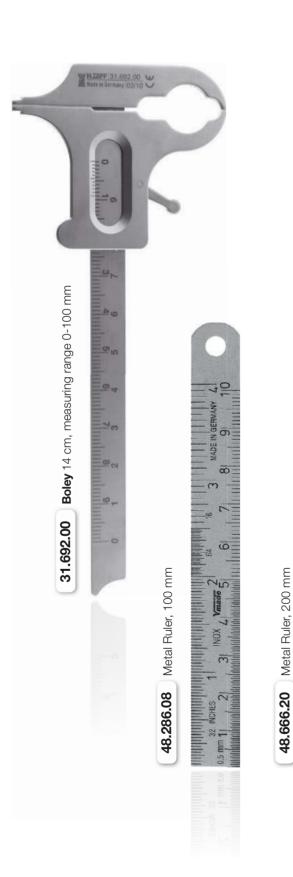



Bone Caliper



31.691.13

Bone Caliper for measuring the maxillary bone, radial scaling on the shanks of the ring handles, 13 cm



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

07-38 Implantology

+49 (0) 74 64 / 98 88 0

Palatal Knife

acc. to Dr. med. dent. Iman Mizani, MS

The novel Palatal Knife offers an innovative alternative to the conventional scalpel for the preparation of connective tissue graft.

The special design of the instrument promotes faster and safer graft removal. At the same time, the risk of injury to the palatine artery and perforation of the palatal flap is minimized.

Special features:

- angled cutting edge, perpendicular to the palatal bone
- ergonomic, angled instrument neck / shaft
- depth gauge (graduation) for precise dimensioning

Advantages over conventional removal methods:

- enhanced safety through reduced risk of injury to the palatine artery and perforation of the palatal mucosa
- simple and ergonomic handling
- fast, precise preparation of the graft
- consistently uniform thickness of the connective tissue graft
- abrading work and cutting in difficult-to-reach places



46.040.15

Palatal Knife acc. to Dr. med. dent. Iman Mizani, MS

Application:



(1) Singular palatal incision and formation of a flap



(2) Preparation to gain connective tissue, using the instrument



(3) Dissection of the prepared connective tissue below the flap, removal of connective tissue as soon as the base is detached from the palatal bone



zepf-dental.com

Implantology 07-39

Implant Guide

for the posterior tooth region, according to Wiedemann

This method quickly and effectively finds the optimal position for the implants in the posterior region. Here, a standard tooth width is assumed. Premolars 8 mm, molars 10 mm, so 1/2 premolar = 4 mm, 1/2 molar = 5 mm

The standard tooth widths used are neither scientifically nor individually 100% correct, but these values deliver highly usable implant positions particularly on edentulous jaws.












STRI HIZI

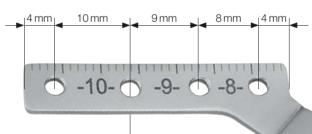

Scale 2:1 Drilled holes: Ø 2.4 mm


Distance between drilled holes

- 8 mm: From the center of one premolar to the center of the next premolar (1 x 4 mm + 1 x 4 mm), e.g. center of number 4 to center of number 5.
- 9 mm: From the center of one premolar to the center of a molar (1 x 4 mm + 1 x 5 mm), e.g. center of number 5 to center of number 6.
- 10 mm: From the center of one molar to the center of the next molar (1 x 5 mm + 1 x 5 mm), e.g. center of number 6 to center of number 7.

If no premolar is available as a starting point then a canine can also be used. For this, a distance between the mesial end of the working part and the first hole of exactly 4 mm was chosen (1/2 premolar width).

10.0.31 31.683.00

Drilling Template acc. to Wiedemann

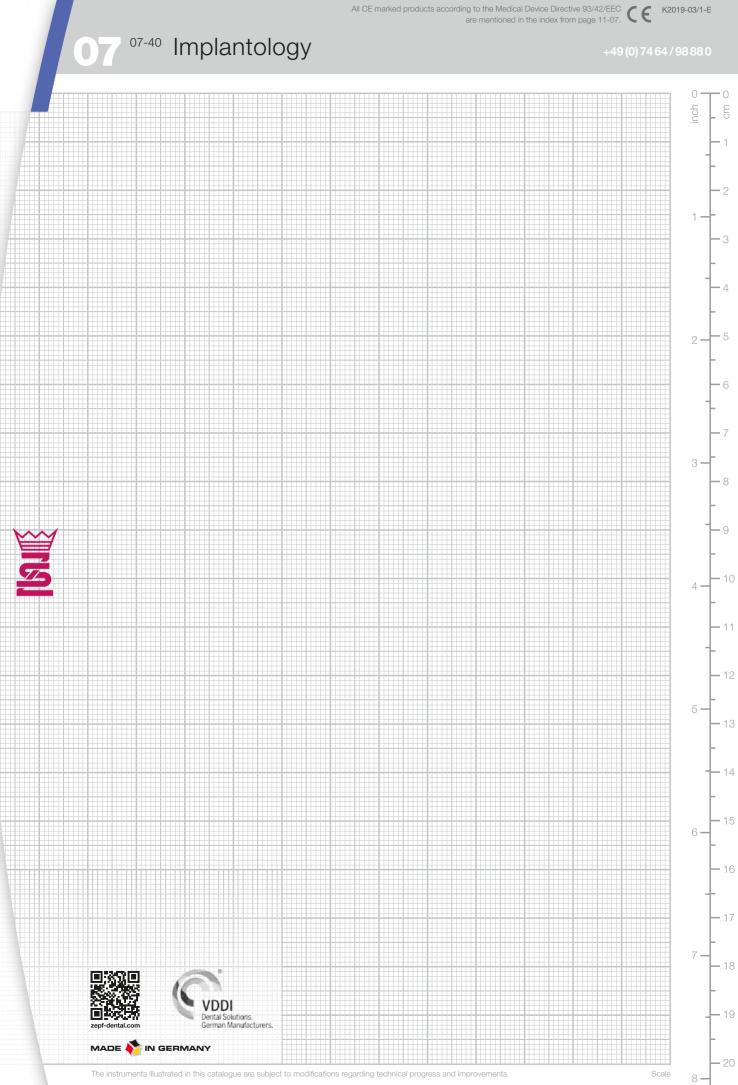



IN

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁸⁻⁰² Microsurgery

+49 (0) 74 64 / 98 88 0

2 NEW **ZEPF** Tunneling Instruments!

Tunneling Instruments with a new angle

> By request of several users, the modified **DONK** Tunneling Instruments from **HELMUT ZEPF** have now been supplemented with two new instruments. The instruments curved beyond the working tip allow even better access, especially in the posterior tooth region. Available in two sizes, depending on the extent of tunneling, the user can now select the ideal instrument for his / her purposes.



consisting of: 1/3 Washtray, Tunneling Instruments
1 upper jaw 46.040.01,
2 lower jaw 46.040.02,
3 upper /lower jaw combination 46.035.20



46.040.03



46.040.04

Tunneling Instrument # 4, 2.5 mm, 45° angled













reddot design award winner 2010

zepf-dental.com

46.040.30

Set for tunneling technique

with 3 Tunneling Instruments like Set 46.040.00, Micro Surgical Scalpel Handle 46.013.00Z and Periosteal Elevator 41.864.30 (**ZEPF**-Line, round-tip 2.8 mm, lance-tip 2.4 mm)



In microsurgery, **HELMUT ZEPF GOOR** Tunneling Instruments find their application in the preparation of flaps or subsequent reconstructions of the alveolar ridge or for root coverings with a connective tissue graft. The instruments allow a minimally invasive tunneling preparation to avoid large openings. Due to the fine shape delicate tunneling incisions in the tissue are possible.

Microsurgery 08-03



ISU

⁰⁸⁻⁰⁴ Microsurgery

+49(0)7464/98880

P

4/0 - 6/0

Double-Action Micro Forceps, transmitted, **ZEPF-**Line,

22.830.17

17.5 cm, 1 x 2 teeth, thread plate 10 mm, jaw width 0.6 mm, SpinLock

4/0 - 8/0

41.017.17 Double-Action Micro Needle Holder, transmitted, ZEPF-Line,

17.5 cm, tungsten carbide, serrated, jaw width 0.6 mm, SpinLock



What is the ZEPF SpinLock?

The parallel lock known from standard needle holders has been replaced with the new SpinLock technology. This avoids that the suture material gets caught up on the needle holder.



The **HELMUT ZEPF** Double-Action Instruments are consisting of a Micro Needle Holder and a pair of Micro Forceps.

The instruments were technically modified in the region of the instrument lock. The usual parallel screw lock has been replaced by a new axially turned lock to reliably prevent the suture material from sticking to the needle holder during knotting.

Advantages of the Double-Action Instruments

- double transmission to allow tactile handling
- made of special stainless steel
- needle holder with tungsten carbide insert to guarantee a long service life
- due to the round shape, the rotation is considerably facilitated, in particular during suturing, contrary to usual flat micro needle holders
- the turned design prevents threads from getting stuck

zepf-dental.com

Microsurgery 08-05



ZEPF Micro Scissors

Onyx-coated scissors offer a 3-5 times higher surface hardness. In combination with the "Supercut" grinding, this guarantees an extremely long product life and application as well as a very high precision and wear resistance. The extraordinary surface smoothness is leading to an easy slide of the scissor blades even under highest strain.

Furthermore, the anti-glare surface avoids disturbing light deflections. The extremely smooth surface prevents adhesion of proteins.



⁰⁸⁻⁰⁶ Microsurgery

+49 (0) 74 64 / 98 88 0

Suture Removal Scissors acc. to Dentist Beck



The newly developed **HELMUT ZEPF** Suture Removal Scissors are combining two functions in one instrument.

Sectioning and Retaining

The curved micro scissors won recognition for periodontal microsurgery. They are qualified for controlled cuts in the soft tissue and their main task is the sectioning of the suture (ill. 1).

They are curved for an ideal access to all oral regions. One blade of the scissors is micro-serrated to prevent the soft tissue and the thread from slipping off (ill. 2).

The new trademarked gripping function allows the scissors to be used for the sectioning of the suture and subsequent thread removal without requiring a second instrument (ill. 2).







46.319.17N

Suture Removal Scissors with retaining function for suture removal by Dentist Beck, micro-serrations, sharp/sharp, **ZEPF**-Line, curved, SpinLock, 17.5 cm Needle Holder acc. to Dr. Kirsch



Needle Holder by Dr. Kirsch, lock, double spring, SpinLock, 17.5 cm, TC





zepf-dental.com

Macro / Micro Needle Holder



4/0 - 8/0

41.201.15TC

41.010.17TC-M Macro Needle Holder 18 cm, TC macro bit 11 x 2.0 mm, straight, **ZEPF**-Line, titanium, lock

What is TC ?

TC stands for "Tungsten Carbide", a material whose superior strength wear resistance and hardness are its major properties that distinguish it from conventional materials.

Micro Needle Holder ZEPF-Line, with lock and protected inner spring, SpinLock, TC



41.201.15TC stainless steel, 16 cm **41.201.17TC** stainless steel, 17.5 cm





Hold'n'Cut by PD Dr. Weng, combined with scissors, SpinLock, TC



The front part of the Hold'n'Cut Micro Needle Holder holds the end of the needle when entering the flap.



The front part of the needle holder, together with the micro surgical tweezers, holds the thread ends when knotting.



The back part of the Hold'n'Cut Micro Needle Holder offers scissors for the cutting of the thread without changing the instrument or needing any additional scissors.

zepf-dental.com

Microsurgery 08-09



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁸⁻¹⁰ Microsurgery

+49 (0) 74 64 / 98 88 0



Micro Forceps with Diamond Coating

Some forceps can also be ordered with diamond coated tips for better grip.



CC All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

Microsurgery 08-11

•

ImpacTray

acc. to PD Dr. Weng, Starnberg

The ImpacTray acc. to PD Dr. Weng makes micro as well as macro surgical operations possible in implantology, periodontology and augmentation surgery.

The amount of necessary instruments is reduced to a minimum by developing and putting together an efficient, mainly double-ended and partially exchangeable instrument set. 6666666666

The set composition is illustrated on the following two pages.





⁰⁸⁻¹² Microsurgery

ImpacTray acc. to PD Dr. Weng, Starnberg

The ImpacTray Set

24.971.00

incl. washtray consists of:

K2019-03/1-E



46.035.05 PapillEx Papilla Elevator acc. to PD Dr. Weng, Starnberg

The blunt working end of the PapillEx has a lenticular shape and allows gentle elevation of the tip of the papilla by turning the instrument while positioned adjacently to the cervical part of the tooth.

The sharp working end, which is slightly bigger, is used to remove the periosteum from the bone along the sulcular or vertical incision.

Both working ends are exchangeable and can be removed from the instrument shank if necessary.

5/0 - 8/0

yellow, exchangeable

24.201.05L

blunt





24.208.03L

black, exchangeable

24.210.01L



⁰⁸⁻¹⁴ Microsurgery

+49 (0) 74 64 / 98 88 0

 (ϵ)

K2019-03/1-E

Papilla Elevators



46.035.05 PapillEx Papilla Elevator by PD Dr. Weng, Starnberg

The blunt working end of the PapillEx is lentiform and allows gentle elevation of the tip of the papilla by turning the instrument while positioned adjacently to the the cervical part of the tooth.

The sharp working end, which is slightly bigger, is used to remove the periosteum from the bone along the sulcular or vertical incision.

Both working ends are exchangeable and can be removed from the instrument shank if necessary.





Micro Scalpel Handles ZEPF-Line, 13 cm



Micro Scalpel Blades for Micro Blade Holders, supplied in packs of 25 pieces



zepf-dental.com

ZEPF Soft Tissue Micro Instrument Basic Set


24.967.05

ZEPF Soft Tissue Micro Instrument Basic Set

85.180.00

Incl. washtray 1/1, with 2 instrument supports and 1 longitudal instrument retainer, dimensions: 275 x 178 x 24 mm

containing:



Tissue Forceps, straight, stainless steel, **ZEPF**-Line, with guide pin, 1 x 2 teeth, 17.5 cm

(2) 41.200.17TC-K

Needle Holder by **Dr. Kirsch**, straight, TC, lock, double spring, SpinLock, 17.5 cm



Raspatory, **ZEPF**-Line




Suture Removal Scissors with micro-serrations, sharp/sharp, curved, **ZEPF**-Line, stainless steel, 17 cm

(5) 46.013.00Z

Micro Surgical Scalpel Handle, **ZEPF**- Line, light version, titanium, 13 cm



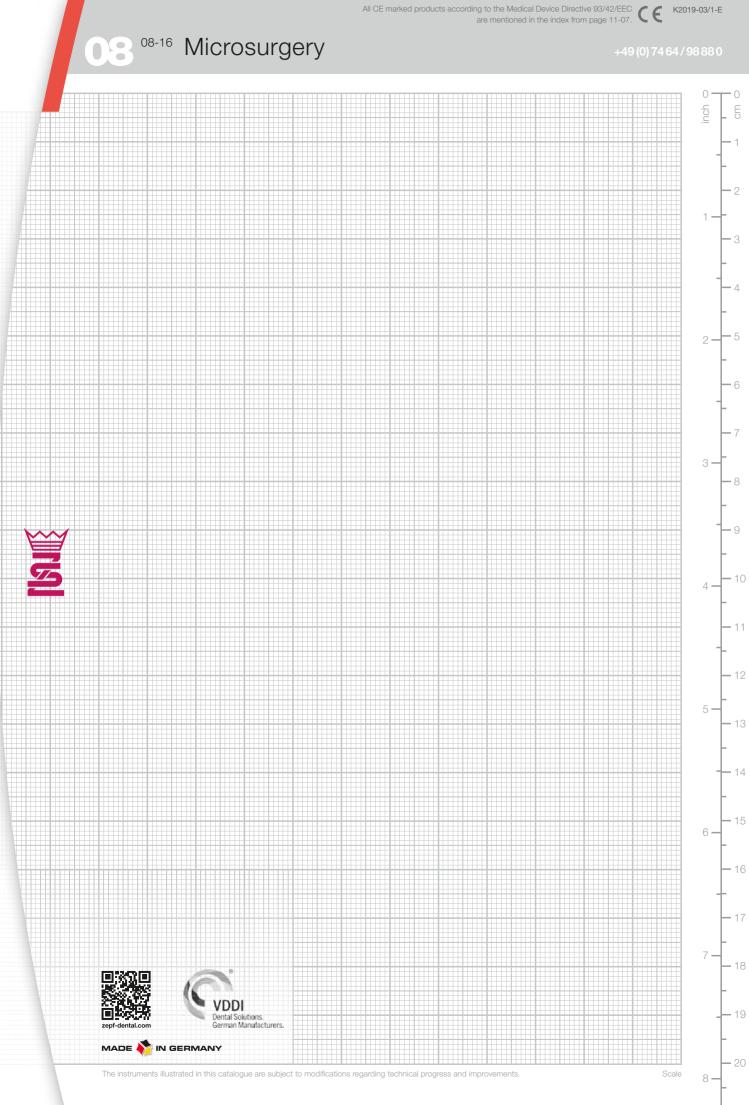

K2019-03/1-E

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Crown Instruments 09-01

5

ZEPF Crown-Spreading Pliers

The **HELMUT ZEPF** Crown-Spreading Pliers are perfectly designed for the spreading of crowns without pressure on the root and neigbour tooth.

The spreadding function of these pliers guarantee a safe and anatomical correct application. The power is not anymore transfered to adjacent teeth,

roots or the jaw as with conventional crown spreading pliers.

19.277.01Z

Crown-Spreading Pliers by Bauer, modified DBGM, 14.5 cm

09-02 Crown Instruments

+49 (0) 74 64 / 98 88 0

Universal Forceps

These **HELMUT ZEPF** All-purpose Pliers should be on hand at any treatment unit. They may be used for securely grasping temporary plastic crowns, bridges, nerve instruments, stuck matrices, fixing inlays, setting interdental wedges, etc., and may be used on both upper and lower jaws.

Their tungsten carbide steel jaws provide a secure grip.



ZEPF Tele-Grip Easy and thus precise adjustment!

There is always a demand for a precise and above all a sensitive adjustment of a Tele-Grip, to avoid a high tension (damage caused by deformation) in critical situations.

The previous function was only partly given, especially in bigger spreading ranges it was only possible under restrictive conditions. Thus, the durability was affected due to the resulting thread damages.

The **HELMUT ZEPF** Tele-Grip has a movable threaded bearing. As a result, the adjusting screw can be aligned easily and in a most sensitive way throughout the setting range.

gently opening in every position

moveable thread bushings for a gentle



31.182.01

Tele-Grip, Telescope Crown Forceps, curved, exchangeable, 15 cm



Crown-Tractor Crown-Extraction Pliers with interchangeable plastic tips



Adjust the screw on the plier so that it fits nicely over the crown to be removed



After adjusting the plier, tips should be moistened with diamond powder



The crown can now be removed in a safe way

19.274.00

CROWN-TRACTOR Set "Exclusive" Extraction Pliers with thumbscrew detent and retaining spring, 16 cm 20 Plastic Polymer Tips,

10 g DIATRAC adhesive powder

19.274.01

CROWN-TRACTOR Set "Economical" Extraction Pliers without thumbscrew detent and retaining spring, 16 cm 20 Plastic Polymer Tips, 10 g DIATRAC adhesive powder




19.274.13

Replacement Kit: 10 g DIATRAC adhesive powder and 40 Plastic Polymer Tips



All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. K2019-03/1-E

09-04 Crown Instruments

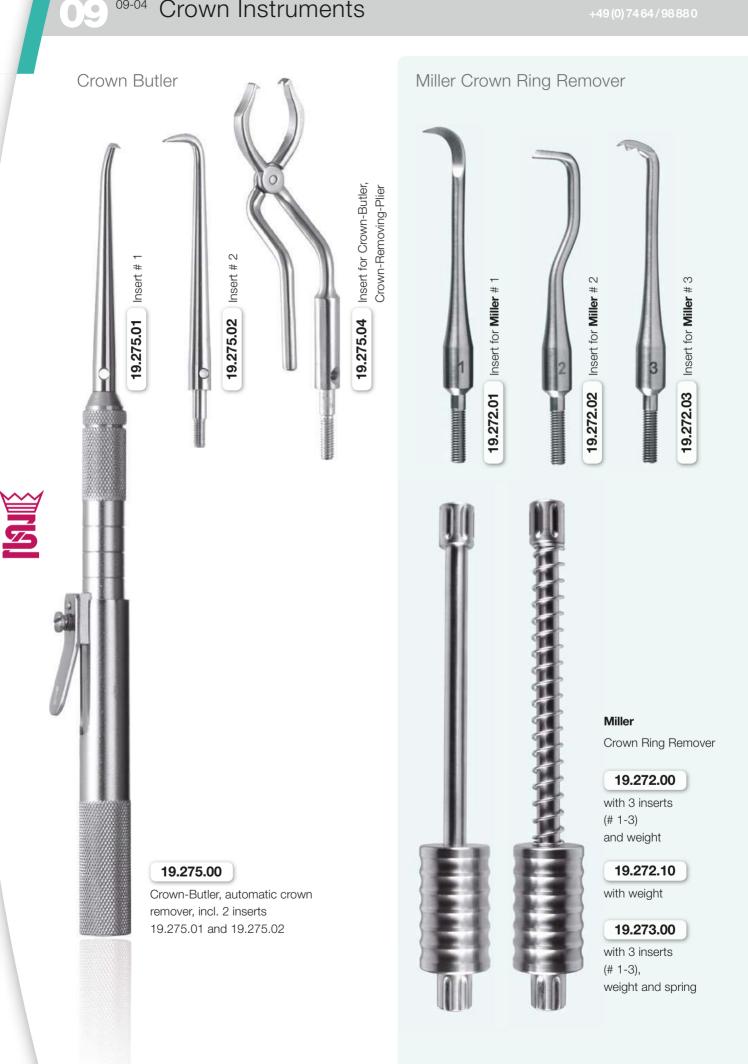



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

⁰⁹⁻⁰⁶ Crown Instruments

+49 (0) 74 64 / 98 88 0



Telecrown-Grip

These Telescoping-Jaw Pliers offer three variation possibilities in one.

Their adjustable and rigid tips have a first-class, anatomically correct friction coefficient.

The design of the contacting surfaces of their diamondtipped jaws significantly extends jaw service life. The choice of configurations allows adapting them to suit patients' anatomies.



31.185.00

Telecrown-Grip,

bilaterally adjustable, 2.35 mm, diamond-tipped jaws with exchangeable, movable tips, incl. Allen Key, 13 cm







Telecrown-Grip, unilaterally adjustable, 2.35 mm, diamond-tipped jaws with

exchangeable tips, 1 movable tip, incl. Allen Key, 13 cm





Telecrown-Grip, rigid, 2.35 mm, diamond-tipped jaws with exchangeable tips, incl. Allen Key, 13 cm

Spare Parts

31.185.10

0 1 pair of diamond-tipped jaws, adjustable, 2.35 mm

31.185.12

2 1 pair of diamond-tipped jaws, rigid, 2.35 mm

31.184.01 Allen Key, SW 1.5

Crown Instruments 09-07

Modeling Instruments – Precision in Perfection


Quality MADE IN GERMANY for the quality-conscious technician.



⁰⁹⁻⁰⁸ Crown Instruments

+49 (0) 74 64 / 98 88 0

Prosthetic Kit

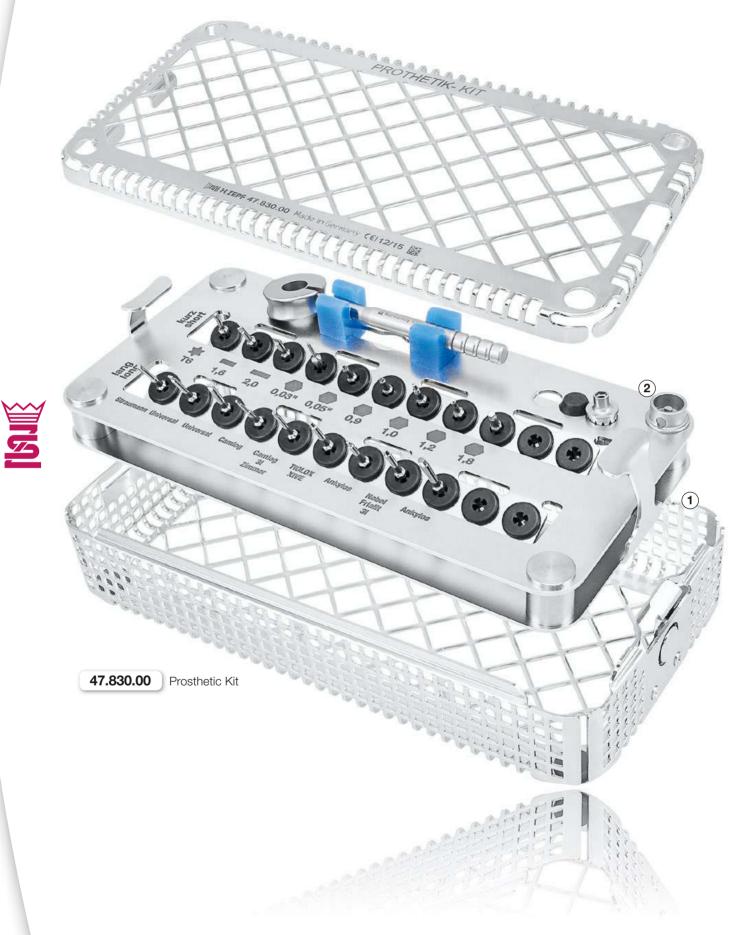

 $(\mathbf{5})$

E

Crown Instruments 09-09

Prosthetic Kit

Every day, you have to loosen all kinds of implant abutments in the practice / in the laboratory? In order to facilitate your work, **HELMUT ZEPF** has created a prosthetic set allowing you to loosen more than 90% of all screws available on the market.

All instruments are numbered and dispose of a RA-HEX connection. This means that these instruments can be used either in a contra-angle handpiece or in a ratchet.

Advantages Prosthetic Kit



In the RA-Hex-Adapter the inserts will be picked up.

Optionally, the finger ratchet can be used with an extension piece. The set can also be completed by a torque wrench which is adjustable from 10-40 Ncm and has a fixation function to deactivate the torque.

The storage tray is made of stainless steel and contains a description of each individual screwdriver in order to facilitate the identification of the tools required for the respective screw. The tray fits into a basket and can be reprocessed reliably according to the RKI guidelines.





RA-Hex Adapter inserted in ratchet. Shown with demounted handle for use as finger ratchet. Information: The RA-Hex-Adapter has a rotating finger rest available (see red arrow).


Among the recessi for two RA-Hex-Adapters a socket for a comfortable removal of the screwdriver inserts from the RA-Hex-Adapter is located.

47.830.00 Complete Prosthetic Kit consisting of:

Shape	Screwdrivers with dental lock	short, 21 mm	long, 26 cm
Σ_{λ}	TORX T6, Straumann, Aesthura	47.832.01	47.833.01
	Universal flat 1.6 mm, narrow	47.832.02	47.833.02
	Universal flat 2.0 mm, wide	47.832.03	47.833.03
\bigcirc	Allen Key SW HEX 0.03'', Camlog	47.832.04	47.833.04
\bigcirc	Allen Key SW HEX 0.05'', Camlog, Sulzer (Zimmer), Semados, Biomet 3I	47.832.05	47.833.05
\bigcirc	Allen Key SW 0.9 mm, IMPLA, TIOLOX, BREDENT, XIVE	47.832.06	47.833.06
\bigcirc	Allen Key SW 1.0 mm, Ankylos	47.832.07	47.833.07
\bigcirc	Allen Key SW 1.2 mm, IMPLA, Nobel Biocare, Frialit, XIVE, IMZ, Biomet 3I	47.832.08	47.833.08
\bigcirc	Allen Key SW 1.8 mm, Ankylos	47.832.09	47.833.09
1	1/3 Washbasket with Lid	8	5.192.50
2	Rack for Prosthetic Kit	4	7.830.01
3	Driver Guide		7.525.50
4	Ratchet with demountable handle for Prosthetic Kit	4	7.525.55
5	Optional Accessory: Torque Wrench (not included in the set)	47	.803.02*

ALL THE TRADEMARKS ARE THE PROPERTY OF THE RESPECTIVE COMPANIES. We assume no liability for deviations due to tolerances of implants.



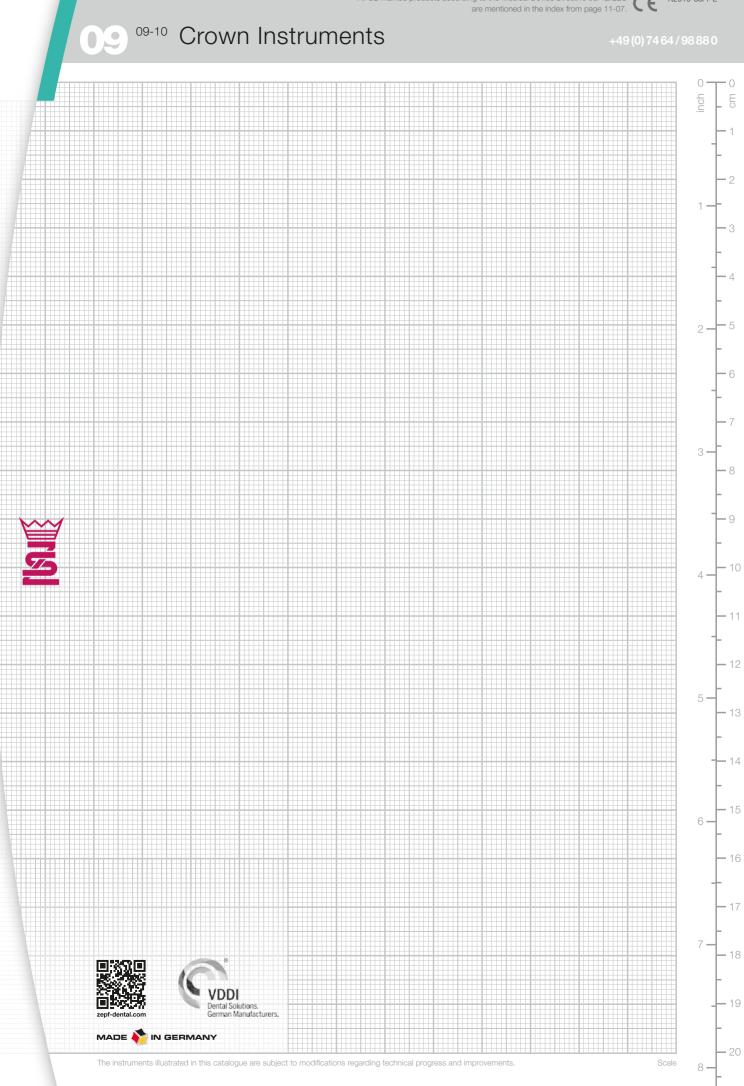

All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07. CE

K2019-03/1-E

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Maintenance 10-01





The Modular Hygiene System

Flexible, efficient and approved safe. The **ZEPF**-Care Universal Silicone Profile allows an easy placement of the instruments after a surgery. For sterilization and cleaning, the instruments are inserted in the profile according to their diameter and are immediately secured.

Additionally, we have equipped the **ZEPF**-Tray and Basket-System with silicone base. Therefore the tray guarantees an anti-slip position and the stacking stability is improved at the same time.

Suitable for standardized sterilization containers, it's available in four different sizes for an ideal working potential. Placesaving, secure and very practical and with a removable lid.













All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

¹⁰⁻⁰² Maintenance

+49 (0) 74 64 / 98 88 0





The **ZEPF**-Care-System increases your efficiency, as you can assemble your trays in a process-oriented way and work accordingly.

You will meet the requirements of the RKI and the accident prevention regulation.

It doesn't matter whether you are cleaning your instruments manually or automatically.




Maintenance 10-03

Profile, high, universal

Advantages

- The meshes of the bottom and the lid are designed in a broad shape. Consequently dead zones are minimized.
- The diagonal profile of the mesh simplifies the identification of the parallel arranged instruments in the profile.
- The meshes on the edge of the tray are designed in a narrow shape and thus enhance the stability of the tray.
- The risk of injury is reduced.

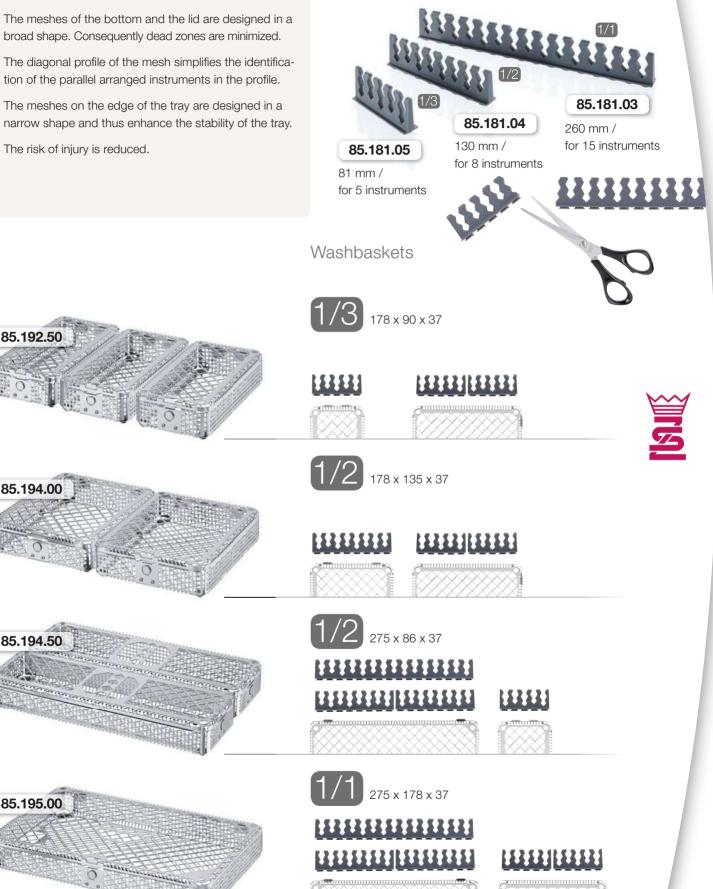

¹⁰⁻⁰⁴ Maintenance

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

+49 (0) 74 64 / 98 88 0

Profile, high, universal (example see picture 1)

intelligent







Arranged in a practiceoriented way

As a result of the high and low configuration of the profile sections, the instruments can be placed in a space-saving way and can be removed easily.

It is possible to place two instruments above each other in one profile section. Contact of the instruments should be avoided in order to prevent contact corrosion.

Tip:

The following instrument combinations are **possible** should they contact each other:

- plastic / plastic
- plastic / metal ✔
- titanium / titanium
- titanium / metal

In case of contact, the following instrument combination is **not possible**:


metal / metal X

The modular concept of the three different lengths can be tailored according to your request.

The 'universal profile' is compatible with the 'low profile' in order to ensure a secure hold of different instrument diameters and variations.

For special cases, we recommend the assembly of our press pad in the lid.

There are no limits set regarding design of your personalized tray.

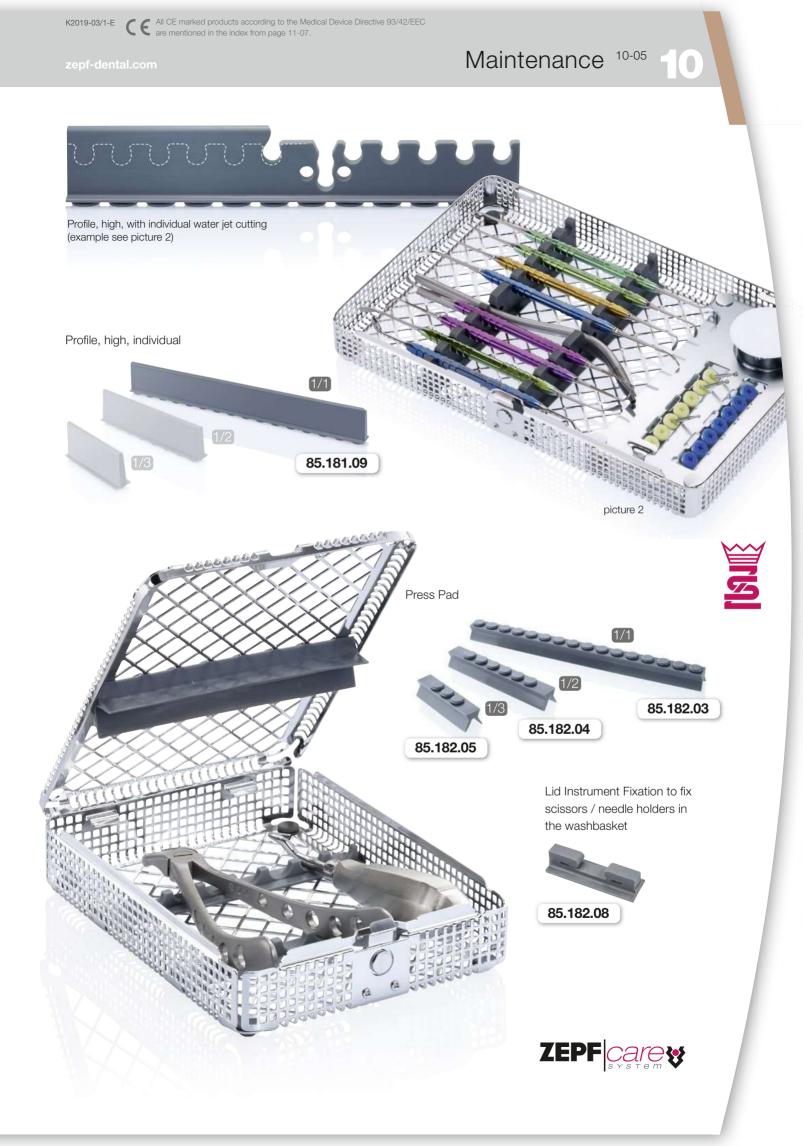

¹⁰⁻⁰⁶ Maintenance

Ś



Maintenance 10-07



Aluminium Sterilization Container in 5 Sizes


Through the integrated filter in the lid and the base the Sterilization Containers are suitable for all steam sterilization methods:

- fractionized vacuum method
- fractionized steam method
- gravitation method
- pre-vacuum method

Different dimensions and stackability allow easy handling and optimal organization. The containers can be used for storing sterile goods and also for disposing contaminated instruments.

The newly developed latch system prevents accidental opening of the container and assures a simplified handling for the sterilization preparation.

The optimized sealing system assures a safe fixing of the filter.

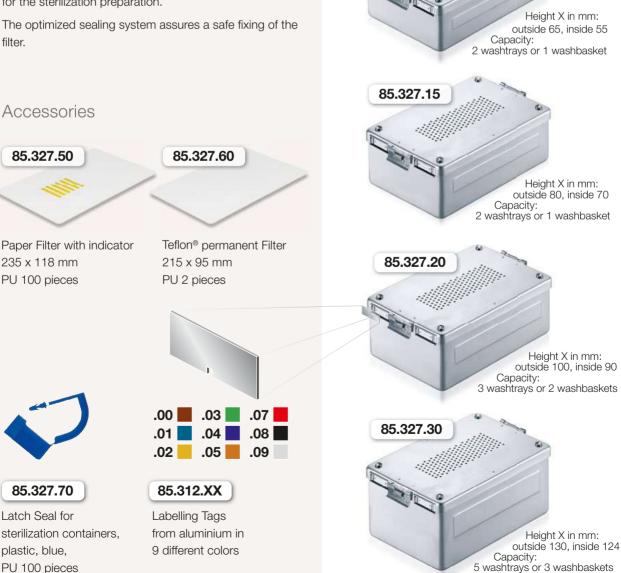



Bottom and lid is perforated, optimized latch system, incl. 2 long-term textile filters Dimensions in mm:

Height X in mm:

outside 40, inside 35

1 washtray or 0 washbaskets

Capacity:

Outside:

85.327.00

85.327.10

Width 310 / Depth 190 / Height X Inside:

Width 280 / Depth 182 / Height X

10-08 Maintenance

 (ϵ)

K2019-03/1-E

Dental-Tray Cassette

All Dental-Tray Cassettes are compatible to our Washtray and Washbasket System, shown on pages 10-02 to 10-04.



85.142.20

Norm-Tray-Cover 1/2, non perforated, 180 x 140 x 25 mm

All CE marked products according to the Medical Device Directive 93/42/EEC

are mentioned in the index from page 11-07.

85.142.10

Norm-Tray-Bottom 1/2, perforated, 180 x 140 x 19 mm

85.145.00

Norm-Tray-Cover 1/1, non perforated, 280 x 180 x 25 mm

85.150.00

Norm-Tray-Bottom 1/1, perforated, 284 x 183 x 17 mm

85.140.00

Norm-Tray-Bottom 1/1, non perforated, 284 x 183 x 19 mm



Drill holder inserts, assorted in 9 colors (5 pieces ea. per packing unit). 85.183.40 with bigger inner diameter for piezo instruments, available only in black color.

÷


+



Brushes with nylon bristles

PROBLEM: Metal brushes They destroy the passive layer of the instrument surface!

SOLUTION: Brushes with nylon bristles

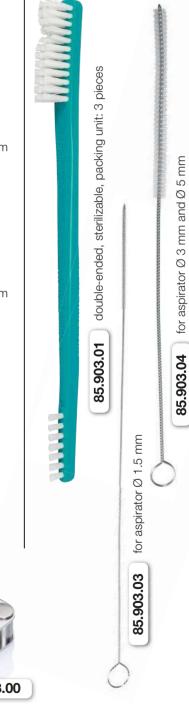

incl. mixing cup with lid and silicone

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

Maintenance 10-09

ZEPF Medicine Cups

85.252.25

Medicine Cup, stainless steel, Ø 60 mm x 27 mm high, 25 ccm



Mixing Cup, stainless steel, with plastic lid, Ø 4 cm



85.251.04

Medicine Cup, stainless steel, with plastic lid, Ø 40 mm x 30 mm high

85.251.03

Medicine Cup, stainless steel, with plastic lid, Ø 40 mm x 25 mm high, usable on both sides





24.950.12 Oil Pen, 12 ml

Paraffinum Perliquidun 24.950.10 Parattin OI / M

> HELMUT ZEPF zept denta

24.950.10 Dispensing bottle, 50 ml

All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

¹⁰⁻¹⁰ Maintenance

+49 (0) 74 64 / 98 88 0

F

K2019-03/1-E

Universal Toolbox for the ZEPF CMF SYSTEM

The universal tool box is used for storing the tools for the sets CMS + ARCS. The tool box offers enough space for the following items:

- Screwdriver handle, big and small, each with dental connection, in the new optimized **ZEPF**-Design. They have a socket for exchangeable blades of all different diameters. The use of the handles is easy and intuitive while changing the blades.
- The blade holder allows an extra secure fixing of the screw heads on the blade insert.
- The pilot drills and the slide hole drill both have a graduation to allow a safe depth orientation.
- The inserting assistant is used for areas with tight space conditions.
- The Pin Applicator 47.950.02 which fits in the screwdriver handles completes the set for fastening foils and membranes.

47.950.02

Pin Applicator with dental connection



Screw Rack for the Universal Toolbox


The Screw Racks are available in the following configurations:

- 85.540.60 Screw Rack Ø 1.0 / 1.2 mm each 4 rows
 + 2 rows Ø 1.5 mm to accommodate 5 screws
- 85.540.65 Screw Rack Ø 1.2 / 1.5 mm each 5 rows to accommodate 5 screws

The packing unit for the screws is 5 pieces.

An easy identification of the screws is guaranteed by using the length markers in the tray.

The colored pin with length marking is assigned to the respective screw diameter, thus allowing the determination of the screw length and a clear lot traceability in the box.



85.540.65

Screw Rack Ø 1.2 / 1.5 mm each 5 rows to accommodate 5 screws



47.501.03

CMF-Box for Screw Systems Ø 1.0 mm, Ø 1.2 mm and Ø 1.5 mm

85.540.60

Screw Rack Ø 1.0 / 1.2 mm each 4 rows + 2 rows Ø 1.5 mm to accommodate 5 screws

K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Maintenance 10-11

Washbasket for the **ZEPF** CMF SYSTEM

Following the Zepf-Care Series, the modularly composable components for the **ZEPF** CMF SYSTEM were developed, offering a washbasket with appropriate combination options.

The actual tools can be organized depending on the desired diameter.

This guarantees an RKI compliant reprocessing of the CMF SYSTEM.

85.195.00

Washbasket 1/1 as rack for the remaining components

Accessories for the Washbasket

Boxes Dimensions 85 x 75 x 22 mm (L x W x H)

47.503.53

Screw and Pin Box for 2 x 5 screws Ø 1.2, 1 x 5 screws Ø 1.5, 10 membrane pins and a small storage space for instruments, membranes, bone plates etc.


47.503.50

Screw and Pin Box for 3 x 5 screws Ø 1.0, 10 membrane pins and a small storage space for instruments, membranes, bone plates etc. 47.503.10

Box for Screws Ø 1.0 mm




Box for receiving e.g. titanium plates

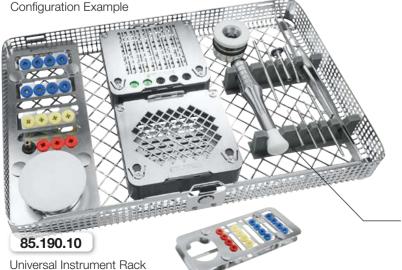

85.251.04

Mixing Cup with lid, stainless steel, Ø 4 cm

Profile for instruments with individual water jet cutting

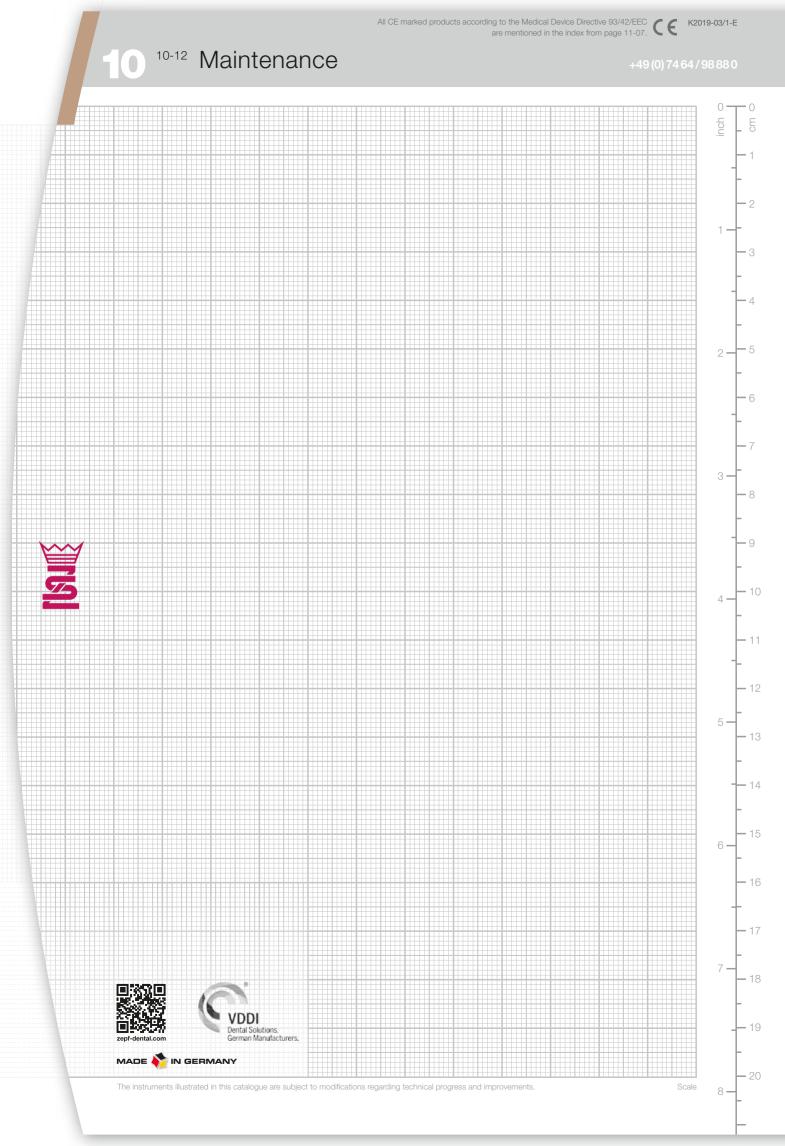



All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻⁰² Alphabetical Index

+49(0)7464/98880

Α			
Adenoid Curette			07-19
Adson Forceps			06-05
Adson Micro Forceps			06-04
Allen Key		06-30.	09-09
Allis Tissue Forceps		00 00,	06-06
All-purpose Forceps			09-02
All-purpose Handles M2.5			02-05
All-purpose Pliers			04-27
Alveolar Ridge Measuring Caliper			07-37
Amalgam Gun			04-08
Anatomic Forceps		03-36,	06-02
Anatomical Plate Forceps			03-36
Anterior VGO Ost-Set			07-16
Antrum Probe			06-42
Apical Root Elevator			05-59
Approximal Desmotome			05-50
Arkansas, Original Sharpening Ston	е		03-32
Articulating Forceps			04-24
Aspirator	06-40	, 07-27,	
Aspirator with Luer Connector			03-36
Atraumatic Surgical Forceps			06-04
Atraumatic Tissue Forceps		06-03,	08-10
ATTIN Compo Knife			04-06
Augmentation Kit		07-32 -	
Augmentation Material Applicator			07-34
В			
Back Action Chisel		03-31,	07-11
Backhaus Towel Clamp			06-06
Ball-shaped Plugger			04-09
Bauer Crown-Spreading Pliers			09-01
Beck Atraumatic Forceps			06-03
Beck Extracting Forceps		05-27 -	
Beck Root Elevator			05-53
Beck Suture Removal Scissors			00 00
			08-06
Beebee Crown Scissors			06-36
Beebee Crown Scissors Bein Elevator			06-36 05-52
Beebee Crown Scissors Bein Elevator Benex Extraction		05-01 -	06-36 05-52 05-06
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor			06-36 05-52 05-06 05-05
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps			06-36 05-52 05-06 05-05 06-25
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik			06-36 05-52 05-06 05-05 06-25 03-01
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap		05-03,	06-36 05-52 05-06 05-05 06-25 03-01 03-03
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set	00.00	05-03, 03-06 -	06-36 05-52 05-06 05-05 06-25 03-01 03-03 03-07
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle	02-02,	05-03, 03-06 - 03-02 -	06-36 05-52 05-06 05-05 06-25 03-01 03-03 03-07 03-03
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle	02-02,	05-03, 03-06 -	06-36 05-52 05-06 05-05 06-25 03-01 03-03 03-03 03-03 03-03
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert	02-02,	05-03, 03-06 - 03-02 - 03-02 -	06-36 05-52 05-06 05-05 06-25 03-01 03-03 03-07 03-03 03-03 03-03
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette	02-02,	05-03, 03-06 - 03-02 - 03-02 - 03-06 -	06-36 05-52 05-06 05-05 03-01 03-03 03-03 03-03 03-03 03-03 03-03
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 05-05 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler Blade Holder		05-03, 03-06 - 03-02 - 03-02 - 03-06 -	06-36 05-52 05-06 05-05 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-30
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder Drop-Control		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07 03-07 03-07
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-30 06-27 06-24
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-30 06-27 06-24 06-26
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder Jorop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-30 06-27 06-24 06-26 07-37
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder JD Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone- & Alveolotomy File		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 08-14 06-30 06-27 06-24 06-26 07-37 06-43
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone- & Alveolotomy File Bone Caliper		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 08-14 06-30 06-27 06-24 06-26 07-37 06-43 07-37
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone- & Alveolotomy File Bone Caliper Bone Crusher		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07 08-14 06-30 06-27 06-24 06-26 07-37 06-43 07-37
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone- & Alveolotomy File Bone Caliper Bone Crusher Bone Cutting Forceps		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-05 06-25 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07 08-14 06-20 06-27 06-24 06-26 07-37 06-43 07-37 07-21 06-26
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone Caliper Bone Cusher Bone Cutting Forceps Bone Fitting Set		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-30 06-27 06-24 06-26 07-37 06-43 07-37 07-21 06-26 07-11
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Sa Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone - & Alveolotomy File Bone Caliper Bone Crusher Bone Cutting Forceps Bone Fitting Set Bone Holding Forceps		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-26 07-37 06-24 06-26 07-37 06-43 07-21 06-26 07-11 06-26
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set bionik Mouth Mirror Handle bionik Reduction Insert bionik Sickle Curette bionik Sickle Curette bionik Sickle Scaler Blade Holder Blade Holder 3D Blade Holder 3D Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Böhler Bone Rongeur Forceps Böhler Bone Rongeur Forceps Boley Sliding Caliper Bone- & Alveolotomy File Bone Caliper Bone Crusher Bone Cutting Forceps Bone Fitting Set Bone Holding Forceps Bone Mill		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07 08-14 06-26 07-37 06-24 06-26 07-37 07-21 06-26 07-11 06-26 07-22
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set Bionik Gracey M5 Prophylaxis Bade Holder Blade Holder Blade Holder SD Blade Holder SD Blade Holder Drop-Control Blumenthal Bone Rongeur Forceps Boher Bone Rongeur Forceps Bone Caliper Bone Caliper Bone Cutting Forceps Bone Fitting Set Bone Holding Forceps Bone Mill Bone Mill Forceps		05-03, 03-06 - 03-02 - 03-06 - 03-06 - - 06-30,	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 03-07 03-07 03-07 03-07 03-07 06-24 06-26 07-37 06-43 07-21 06-26 07-21 06-26 07-21
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Set Biade Holder Curette bionik Sickle Scaler Blade Holder Soler Blade Holder 3D Blade H		05-03, 03-06 - 03-02 - 03-02 - 03-06 - 03-06 -	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 03-07 08-14 06-26 07-37 06-24 06-26 07-37 06-43 07-37 06-24 07-21 06-26 07-21 06-26 07-21 06-26
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey Science Set Bone Caliper Bone Cusher Bone Cutting Forceps Bone Fitting Set Bone Holding Forceps Bone Mill Bone Mill Forceps Bone Rongeur Forceps Bone Rongeur Forceps Bone Scraper		05-03, 03-06 - 03-02 - 03-06 - 03-06 - - 06-30,	06-36 05-52 05-06 03-01 03-03 03-07 03-03 03-03 03-03 03-07 03-07 03-07 03-07 03-07 03-07 03-07 03-07 06-24 06-26 07-37 06-24 06-26 07-21 06-26 07-21 06-26 07-21 06-26 07-21
Beebee Crown Scissors Bein Elevator Benex Extraction Benex Pole Extractor Beyer Bone Rongeur Forceps bionik bionik End Cap bionik Gracey M5 Prophylaxis Set bionik Gracey M5 Prophylaxis Bionik Gracey M5 Prophylaxis Blade Holder Curette bionik Sickle Scaler Blade Holder Socaler Blade Holder 3D Blade Holder 3	06-27	05-03, 03-06 - 03-02 - 03-06 - 03-06 - - 06-30,	06-36 05-52 05-06 03-01 03-03 03-03 03-03 03-03 03-03 03-03 03-07 03-07 08-14 06-26 07-37 06-24 06-26 07-37 06-43 07-21 06-26 07-11 06-26 07-21 06-26 07-21 06-26 07-21 06-26 07-05 07-05

Bowdler-Henry's Rake Bowl Bridges and Crowns Removing Pliers Brozio Anatomical Plate Forceps Brush Brush Holder Brush Holder Brush Holder CompoSMOOTH Bur Stand	3	04-04 -	06-12 06-41 09-05 03-36 10-08 04-22 04-05 07-20
С			
Cannula, Syringe Cartridge Syringe Carving Instrument Cawood-Minnesota Cheek Retractor Cement Spatula Cheek and Lip Rectractor Cheek Retractor / Photography Retra Cheek Retractor Onyx Chisel Chompret Syndesmotome Cleveland Bone Cutting Forceps Cleveland Bone Rongeur Forceps Cleveland Bone Rongeur Forceps CMF System CMF-Box Columbia Universal Curette Compo Knife ATTIN Composite Instrument Composite Instrument	actor	06-10 - 06-09, 07-09, 10-10 - 03-18 - 04-02 - 04-04 -	02-07 06-15 02-07 07-11 05-58 06-26 06-25 10-11 10-10 03-19 04-06 04-05 04-01
Crile-Wood Needle Holder Crown Butler Crown Forceps Crown Holding Pliers Crown Lever Crown Remover automatic Crown Ring Remover Crown Scissors Crown-Extraction Pliers Crown-Extraction Pliers Crown-Spreading Pliers Crown-Tractor Cryer Root Elevator Curette Gracey bionik Curette Titanium		06-36, 03-16 - 03-20 - - 03-20,	06-39 09-04 09-02 09-05 09-05 09-04 09-04 09-03 09-01 09-03 05-61 03-17 -03-21

D

De Bakey Forceps	06-02
Dean Scissors	06-33
Deep Scaling	03-06 - 03-07
Denhart Mouth Retractor	06-11
Dental-Tray Cassette	10-08
Derf Needle Holder	06-39
Desmotome	05-44 - 05-45
Diamond Drill	07-27, 07-29
Diamond-Tipped Jaws	09-06
Diatrac	09-03
Disimpaction Forceps	06-11
Double-Action Instrument	08-04
Dressing Forceps	06-06, 08-10
Drill Rack	10-08
Drilling Sleeve	07-35



Drilling Template07-39Drop-Control® Blade Holder06-27

E	
Easy Contact Point Instrument	04-25
ECO ImplaTool Set	07-01 - 07-04
Elevator	06-23
Elevator for axial luxation	05-57
Elevators	06-19, 06-21
Endo Handle	03-09
Endo Set	03-34 - 03-35
Endodontic Mirror	03-37
Excavator	04-12 - 04-13
Exlog Extracting Forceps	05-33 - 05-36
Exlog RoBa Extracting Forceps	05-37 - 05-40
Extracting Forceps	05-07 - 05-40
Extracting Forceps, American Pattern	05-20 - 05-25
Extraction System Benex	05-01 - 05-06

F

09-07
03-30
06-47
04-02 - 04-05
06-08
04-26
07-35
05-49
05-56
06-02 - 06-05, 08-10
03-36, 06-02
06-03 - 06-04
08-09
06-02 - 06-05
06-44
06-41
03-09

G

•	
Gärtner Root Elevator Gerald Forceps	05-52, 05-58 06-05
Giesenhagen One Step Augmentation & I	mplantation
	07-18 - 07-19
Gillies Forceps	06-05
Gingiva Retractor	06-30
Gingivectomy Knife	03-28 - 03-29
Glickmann Raspatory	06-23
Gluckman	06-46
Goldman-Fox Gingivectomy Knife	03-28 - 03-29
Goldman-Fox Scissors	06-33
Gracey Curette bionik	03-16 - 03-17
Gracey Curette stainless steel	03-24 - 03-25
Gracey M5	03-06 - 03-07
Gracey M5 Prophylaxis Set	03-06 - 03-07
Gracey M5 Titanium Curette	03-21
Gross Dressing Forceps	06-06
Н	

••	
Haemostatic Forceps	06-06 - 06-07
Halstead Micro Haemostatic Forceps	06-07
Halstead-Mosquito Haemostatic Forceps	06-07
Hammer	06-47 , 07-10
Handle bionik M2.5	02-02 - 03-03
Handle bionik M4 x 0.5	02-02
Handle Comparison M2.5	02-03
Handle Comparison M4 x 0.5	03-04
Handle Universal M2.5	02-05

Alphabetical Index 11-03

Handle Universal M4 x 0.5 Hartmann Haemostatic Forceps Heidbrink Root-Splinter Elevator Heidemann Spatula Hemingway Sharp Spoon Hildebrand H-Tool Set Hildebrand Luxation Elevator Hilger Retractor Hirschfeld Periodontic Files Hohl Hildebrand Bone Fitting Set Hold'n'Cut Micro Needle Holder Hollow Cylinder Osteotome H-Tool Set Hygienist Scaler bionik Hygienist Scaler stainless steel Hylin Root Elevator	05-46 05-41 - 05-45 02-05 08-08 05-46	03-02 06-07 05-54 04-11 - 06-20 - 05-47 , 05-48 , 06-08 03-28 07-11 , 08-12 07-12 - 05-47 , 03-22 03-27 05-58
I ID Plug Impac Tray acc. to PD Dr. Weng Implant Guide ImplaTool Set Impression Tray Inlay Forceps Instrument Rack universal Inter-Implanory Wedges Iris Scissors Ivory Ivory Rubber Dam Set Jones Towel Clamp	07-01	03-02 - 08-13 07-39 - 07-04 - 04-20 09-03 07-31 07-10 06-32 04-08 04-21
Joseph Scissors Junior Matrix Retainer		06-32 04-24
K Kaplan Mini Scaler Kapogianni Vestibulum Retractor Kelly Haemostatic Forceps Kelly Scissors Kim Retractor Kirkland Gingivectomy Knife Kirsch Micro Needle Holder Kirsch Plugger Kirsch Sinus Lift Set Kirsch Spoon Klingex Safety Blade Remover Knife, Palatal Kocher Haemostatic Forceps Kocher-Langenbeck Retractor Krastl CompoSMOOTH Krekeler Sliding Caliper	07-23, 07-29 07-30 07-23, 07-29 04-01, 04-04	- 07-31 , 07-31 06-29 07-38 06-07 06-14
L La Grange Scissors Langenbeck Finger Protector Langenbeck Retractor Langenbeck-Ryder Needle Holder Langer Universal Curette Stainless s Laster Special Retractor Lichtenberg-Ryder Needle Holder Ligature Scissors Lindo-Levien Root Elevator Lipcare Mouth Mirror	steel	06-32 06-08 06-15 06-37 03-19 03-26 06-18 06-37 06-35 05-55 02-04 06-24

Locklin Scissors

London College Tweezers



06-34

02-08 - 02-09, 03-36

All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻⁰⁴ Alphabetical Index

+49(0)7464/98880

M5 Deep Scaling Set 03-13 M5 Titanium Curette 03-21 Macro Needle Holder 08-07 Magnetic Stick 03-32 Mathieu Needle Holder 06-37 Matrix Band 04-24 Matrix Retainer 04-24 Matrix Retainer 04-24 Matrix Retainer 06-37 May Cheek and Lip Rectractor 06-10 Maty Suction Tube 07-29 Mayo-Hegar Needle Holder 06-38 McCall Universal Curette 03-18 Mead Hammer 06-47 Medical White Oil 10-09 Meiselbach Sinus Elevator 07-23 Meriam Tweezers 02-08 Merrifield Gingivectomy Knife 03-29 Micro Bade Holder 08-14 Micro Bone Rongeur Forceps 06-24 Micro Instrument Set 08-14 Micro Scalpel Handle 08-14 Micro Scissors 08-05 Micro Sinus Spoon 07-27 Micro Sinus Spoon 07-27 Micro Sinus Spoon 07-27 <th>Luer Bone Rongeur Forceps Luer Connector Luer-Lock Syringe Luniatschek Cotton Plugger</th> <th>3, 06-20 06-24 03-36 06-41 06-42</th>	Luer Bone Rongeur Forceps Luer Connector Luer-Lock Syringe Luniatschek Cotton Plugger	3, 06-20 06-24 03-36 06-41 06-42
Meriam Tweezers02-08Merrifield Gingivectomy Knife03-29Metzenbaum Preparation Scissors06-34Metzenbaum-Fino Scissors06-35Micro Aspirator06-40Micro Bade Holder08-14Micro Bone Rongeur Forceps06-24Micro Forceps08-04, 08-09 - 08-10Micro Instrument Set08-04, 08-09 - 08-10Micro Needle Holder08-04, 08-06 - 08-08, 08-12Micro Scalpel Blade08-14Micro Scissors08-04Micro Scissors08-05Micro Sinus Plugger07-27Micro Sinus Plugger07-27Micro Tissue Forceps06-04Micro-composite Spatula04-07Micro-Mirror03-37Middeldorpf Retractor06-13Miller Root Elevator05-57Milling Part for Bone Mill07-22Mirror for Photography06-45Mirror for Photography06-45Mirror Micro03-37Mixing Cup07-19, 07-27, 07-29, 07-31, 07-33, 10-09Mizani Palatal Knife07-38Mobilization Hook06-13Modeling Instrument09-07Modeling Instrument09-07Modeling Instrument09-07Modeling Instrument09-07Modeling Knife04-15Moth Mirror02-04Mouth Prop06-11Mouth Prop06-11Mouth Prop06-11	M5 Titanium Curette Macro Needle Holder Magnetic Stick Mathieu Needle Holder Matrix Band Matrix Retainer Maty Cheek and Lip Rectractor Maty Suction Tube Mayo-Hegar Needle Holder McCall Universal Curette Mead Hammer Medical White Oil Medicine Cup 06-41	03-21 08-07 03-32 06-37 04-24 04-24 06-10 07-29 06-38 03-18 06-47 10-09 , 10-09
Micro Scissors08-05Micro Sinus Plugger07-27Micro Sinus Spoon07-27Micro Sinus Spoon07-27Micro Tissue Forceps08-09Micro-Adson Forceps06-04Micro-composite Spatula04-07Micro-Halstead Haemostatic Forceps06-07Micro Mirror03-37Middeldorpf Retractor06-13Miller Bone- & Alveolotomy File06-43Miller Crown Ring Remover09-04Miller Root Elevator05-57Milling Part for Bone Mill07-22Mini Friedmann Bone Rongeur Forceps06-25Minror Handle M2.502-03Mirror Micro03-37Mixing Cup07-19, 07-27, 07-29, 07-31, 07-33, 10-09Mizani Palatal Knife07-38Mobilization Hook06-13Modeling Instrument09-07Modeling Knife04-15Mott Mouth Prop06-11Mouth Mirror02-04Mouth Mirror02-04	Meriam Tweezers Merrifield Gingivectomy Knife Metzenbaum Preparation Scissors Metzenbaum-Fino Scissors Micro Aspirator Micro Blade Holder Micro Bone Rongeur Forceps Micro Forceps Micro Friedmann Bone Rongeur Forceps Micro Instrument Set Micro Needle Holder Micro Scalpel Blade	02-08 03-29 06-34 06-35 06-40 08-14 06-24 - 08-10 06-24 08-15 3, 08-12 08-14
Mini Friedmann Bone Rongeur Forceps06-25Mini-Kaplan Scaler03-22Mirror for Photography06-45Mirror Micro02-03Mirror Micro03-37Mixing Cup07-19, 07-27, 07-29, 07-31, 07-33, 10-09Mizani Palatal Knife07-38Mobilization Hook06-13Modeling Instrument09-07Modeling Knife04-15Molt Mouth Prop06-11Mouth Gag06-08Mouth Mirror02-04Mouth Prop06-11	Micro Scissors Micro Sinus Plugger Micro Sinus Spoon Micro Tissue Forceps Micro-Adson Forceps Micro-composite Spatula Micro-Halstead Haemostatic Forceps Micro Mirror Middeldorpf Retractor Miller Bone- & Alveolotomy File Miller Crown Ring Remover Miller Root Elevator	08-05 07-27 07-27 08-09 06-04 04-07 06-07 03-37 06-13 06-13 06-43 09-04 05-57
Müller Retractor 06-08	Mini Friedmann Bone Rongeur Forceps Mini-Kaplan Scaler Mirror for Photography Mirror Handle M2.5 Mirror Micro Mixing Cup 07-19, 07-27, 07-29, 07-31, 07-33 Mizani Palatal Knife Mobilization Hook Modeling Instrument Modeling Knife Molt Mouth Prop Mouth Gag Mouth Mirror Mouth Prop Mucosa Membrane Punch	06-25 03-22 06-45 02-03 03-37 3, 10-09 07-38 06-13 09-07 04-15 06-11 06-08 02-04 06-11 07-20

Nabers Furcation Probe	03-09
Nanopal [®] coating	03-06 - 03-0
Needle Holder	06-37 - 06-39
Needle Holder Lichtenberg	06-3
Needle Holder Micro	08-06 - 08-0
Needle Holder Swedish Mod	
Nerve-Canal Pliers	03-30
New Osteotome Kit	07-06 - 07-0
Norm-Tray Cassette	10-08
0	
Obwegeser Retractor	06-12, 06-1
Obwegeser Soft Tissue Hook	K 06-1
Ochsenbein Periodontal Chis	el 03-30 - 03-3
One Step Augmentation & Im	
Onyx RoBa Extracting Forcer	
Onyx Scissors	06-31 , 08-0
Onyx Xtool	05-42 - 05-4
Osteotome	07-12 - 07-1
Osteotome Kit	07-06 - 07-0
Osteotome Set	07-12 - 07-1
P PA Probe	03-01, 03-08 - 03-1
Palatal Knife	03-01, 03-08 - 03-1
Papilla Elevator	06-30, 08-1
Papillex	06-3
Pear-shaped Plugger	04-0
Pedodontic Extracting Forcer	os 05-26, 05-3
Peet Splinter Forceps	03-37, 04-2
Perforation Raspatory	07-3
Periodontal Chisel	03-30 - 03-3
Periodontal Probe	03-01, 03-1
Periodontal Probe exchangea	
Periodontal Set	03-1
Periodontic Files	03-2
Periosteal Elevator	06-21, 06-2
Periotome	05-49 - 05-5
Periotome, exchangeable ins	erts 05-5
Photography Mirror	06-4
Photography Retractor	02-0
Photography Retractor Onyx	
Pi Series	07-0
Pin Applicator	07-07, 07-33, 10-1
Pin Box	10-1
Pin Membrane Probe	07-3
Plain Milling Cutter	07-1
Plate Forceps	03-3
Plugger	04-08, 07-23, 07-29, 07-3
Posterior VGO Ost-Set	07-1
Potts Smith Forceps	06-0
	05-4
Power Periotome	
Power Periotome	06-33 - 06-3
Power Periotome Preparation Scissors	06-33 - 06-3
Power Periotome Preparation Scissors Press Pad	06-33 - 06-3 10-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor	06-33 - 06-3 10-0 06-2
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set Prophylaxis Set 'Bionik'	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0 03-1
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set Prophylaxis Set 'Bionik' Prophylaxis Set 'M5 Deep Sc	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0 03-1 caling' 03-1
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set Prophylaxis Set 'Bionik' Prophylaxis Set 'M5 Deep Sc Prophylaxis Set 'Universal'	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0 03-1 caling' 03-1
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set Prophylaxis Set 'Bionik' Prophylaxis Set 'Bionik' Prophylaxis Set 'Universal' Prophylaxis Set 'Universal' Prophylaxis-Set 'Gracey'	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0 03-1 caling' 03-1 03-1 03-1
Power Periotome Preparation Scissors Press Pad Prichard Retractor Probe Probe Tip interchangeable Profile Profile, individual Prophylaxis Set Prophylaxis Set 'Bionik' Prophylaxis Set 'M5 Deep Sc Prophylaxis Set 'Universal'	06-33 - 06-3 10-0 06-2 02-10, 03-01, 06-4 02-0 10-02 - 10-0 10-0 03-06 - 03-0 03-1



Alphabetical Index 11-05

Q			Shank Inserts	07-07
QuickFix		03-02	Sharp Spoon	05-50, 06-20
			Sharpening Oil	03-32
R			Sharpening Stone	03-32 - 03-33
Ragnell-Davis Retractor		06-13	Sickle Scaler bionik	03-22 - 03-23
Rake Retractor		06-12	Sickle Scaler stainless steel	03-27
Ramus Retractor	00 10	06-16	Silicone Mouth Gag	80-60
Raspatory	06-19 -		Sinus Elevator	07-23 - 07-31
Raspatory / Periosteal Elevator Ratchet for Prosthetic Kit		06-21 09-09	Sinus Instrument Sinus Lift Set	07-23 - 07-31 07-25 - 07-31
Removing Pliers		09-09 09-05		6-40 , 07-27, 07-29
Rescue-Line		05-15	Sliding Caliper	07-36 - 07-37
Retraction-Thread Plugger		06-42	Small Extracting Forceps	05-26, 05-32
Retractor 02-05, 06-08	- 06-18		Soft Application Insert	04-04
Retractor 30°		06-22	Soft Tissue Hook	06-16
Retractor acc. to Kim		06-11	Soft Tissue Micro Instrument Basic Set	08-15
Retractor and Mouth Mirror		02-06	Spatula	04-10
Retractor double-ended		06-22	Special Curette bionik	03-12 - 03-17
Revolving Chisel Vienna Pattern		05-60	Special Curette stainless steel	03-24 - 03-25
Rhodes Back Action Chisel		03-31	Spencer Scissors	06-35
Ring Applicator		07-19	Spiculum Raspatory	06-23
Ring Breaker		07-19	Spina-Nasalis Retractor	06-17
RoBa Extracting Forceps	05-27 -		SpinLock	08-04
RoBa Pedodontic Extracting Forceps		05-32 06-07	Splint	06-44
Rochester-Pean Haemostatic Forceps Rongeur	06-24 -		Splinter Forceps Spoon 07	03-36 2-23, 07-29, 07-31
Root- and Splinter Forceps	00-24 -	05-17	Spoon 07 Sterilization Container	10-07
Root Canal Explorer		03-38	Sternberg Lip Retractor	06-11
Root Canal Plugger	03-38 -		Stiller Sinus Lift Set	07-28 - 07-29
Root Canal Spreader	00 00	03-38	Storage Box for Pins	07-07, 07-33
	- 05-59		Suction Cannula	06-41
Root Elevator No. 195		05-55	Supercut	06-32
Root-Splinter Elevator		05-54	Surgical Aspirator	03-36, 06-40
Rubber Dam Forceps		04-21	Surgical Scissors	06-36
Rubber Dam Frame		04-21	Suture Forceps	06-02
Rubber Dam Punch Forceps		04-21	Suture Forceps Micro	08-10
Ruler		07-37	Suture Removal Scissors	08-06
Ruskin-Liston Bone Cutting Forceps Ryder Needle Holder		06-26 06-39	Syfrig Benex Extraction System Syringe	05-01 - 05-06 06-41
S			T	
Safety Blade Remover		06-28	Tampon Plugger	06-42
Safety Key	00.00	03-05	Taylor Scaler	03-23
Scaler bionik Scaler stainless steel	03-22 -	03-23	Telecrown-Grip	09-06 09-02
Scalpel Handle		03-27 08-14	Tele-Grip Telescope Crown Pliers	09-05 - 09-06
Scalpel Handle / Blade	06-28 -		Template, Drilling	03-00 - 03-00
Scalpel Handle with scale	00 20	06-29	Tessier Mobilization Hook	06-13
Scalpel Micro		06-29	Test Probe, Acryl	03-32
Schäfer Retractor		06-15		-02 - 06-06, 08-09
Scissors	06-31 -		Tissue Forceps Atraumatic	08-10
Screw Box		10-11	Titanium Curette	03-20 - 03-21
Screw Insert angulated, VGO		07-17	Titanium Milling Part	07-21
Screw Insert straight, VGO		07-16	Titanium Pin	07-33
Screw Inserts		07-07	Tofflemire Matrix Band	04-24
Screw Rack		10-10	Tofflemire Matrix Retainer	04-24
Screwdriver Handle			T D	
		07-07	Tongue Depressor	
		07-07 05-14	Torx	09-09
Seldin Root Elevator		07-07 05-14 05-56	Torx Towel Clamp	09-09 06-06 - 06-07
Seldin Root Elevator Semken Forceps		07-07 05-14 05-56 06-03	Torx Towel Clamp Tower Point Scissors	09-09 06-06 - 06-07 06-35
Seldin Root Elevator Semken Forceps Semken-Taylor Forceps		07-07 05-14 05-56 06-03 06-02	Torx Towel Clamp Tower Point Scissors Towner / Jacquette Scaler stainless stee	09-09 06-06 - 06-07 06-35 0 03-27
Seldin Root Elevator Semken Forceps Semken-Taylor Forceps Senior Matrix Retainer		07-07 05-14 05-56 06-03 06-02 04-24	Torx Towel Clamp Tower Point Scissors Towner / Jacquette Scaler stainless stee Trephine	09-09 06-06 - 06-07 06-35 03-27 07-19 - 07-20
Seldin Root Elevator Semken Forceps Semken-Taylor Forceps Senior Matrix Retainer Senn-Miller Retractor		07-07 05-14 05-56 06-03 06-02 04-24 06-13	Torx Towel Clamp Tower Point Scissors Towner / Jacquette Scaler stainless stee Trephine Tungsten Carbide	09-09 06-06 - 06-07 06-35 03-27 07-19 - 07-20 06-32
Secure-Line Seldin Root Elevator Semken Forceps Semior Matrix Retainer Senn-Miller Retractor Separating Disc Separation Forceps		07-07 05-14 05-56 06-03 06-02 04-24 06-13 07-10	Torx Towel Clamp Tower Point Scissors Towner / Jacquette Scaler stainless stee Trephine Tungsten Carbide Tunneling Instrument	07-19 - 07-20 06-32 08-01 - 08-03
Seldin Root Elevator Semken Forceps Semken-Taylor Forceps Senior Matrix Retainer Senn-Miller Retractor		07-07 05-14 05-56 06-03 06-02 04-24 06-13	Torx Towel Clamp Tower Point Scissors Towner / Jacquette Scaler stainless stee Trephine Tungsten Carbide	09-09 06-06 - 06-07 06-35 03-27 07-19 - 07-20 06-32



¹¹⁻⁰⁶ Alphabetical Index

+49(0)7464/98880

U Universal Crown Scissors Universal Curette bionik Universal Curette stainless steel Universal Forceps Universal Prophylaxis Set Universal Titanium Curette Universal Tweezers	06-36 03-18 - 03-19 03-26 04-27 , 09-02 03-14 03-20 04-27
V Vestibulum Retractor VGO Ost-Set Vienna Revolving Chisel Vise Vollmer Hammer Vollmer Valentin Bone Splitting System	06-09, 06-18 07-14 - 07-17 05-60 03-32 06-47 , 07-10 07-08 - 07-09
W Washbasket Washtray Water Syringe Wax Carver Wedge Applicator Wedges Weng Impac Tray Weng Needle Holder Weng Papilla Elevator WHO Probe Wieder Tongue Depressor Williger Raspatories Winter Root Elevator Wire and Ligature Pliers Wire Cutting Pliers Wire Sizing / Ligature Pliers Wisdom Routurier Extracting Forceps Witzel Root-Splinter Forceps	10-03 10-02 06-41 09-07 07-10 07-10 08-11 - 08-13 08-12 08-14 03-10 06-12 06-19 05-61 06-44 06-44 06-44 05-16 05-16
X Xcision Extracting Forceps Xtool Luxation Elevator Xtool Set	05-07 - 05-19 05-41 - 05-48 05-48
Yildirim Drilling Sleeve	07-35
Z Zaufal-Jansen Bone Rongeur Forceps Zepf, Original Sharpening Stone ZEPF-Care System Zepf-Line Periotome Z-Shape Gracey M5 Prophylaxis Set Z-Shape Handle Z-Shape Sickle Curette Z-Shape Sickle Scaler	06-25 03-33 10-01 - 10-07 05-51 03-06 - 03-07 02-01 03-06 - 03-07 03-06 - 03-07



Numerical Index 11-07

Numerical Index Pages 11-08 to 11-19

All medical devices according to the Medical Device Directive 93/42/EEC are marked with CE in the numerical index. All CE marked medical devices that have to be provided with the notified body are marked with * next to the CE mark, in the numerical index. The notified body is available through our latest valid certificates. These are available per request or download from **zepf-dental.com**.



¹¹⁻⁰⁸ Numerical Index

+49(0)7464/98880

08.902.031HF	07-29	CE*
08.906.014C	07-27	CE*
08.906.016C	07-27	CE*
08.906.018C	07-27	CE*
08.906.023C	07-29	CE*
08.906.029C	07-29	CE*
08.910.01	07-20	C€*
08.910.02	07-20	CE*
08.910.03	07-20	C €*
08.910.04	07-20	C €*
08.910.05	07-20	C €*
08.910.06	07-20	(€*
08.910.07	07-20	C €*
08.910.08	07-20	CE*
08.910.08F	07-19	CE*
08.910.08S	07-19	CE*
08.910.09	07-20	CE*
08.910.09F	07-19	CE*
08.910.09S	07-19	CE*
08.910.10	07-20	CE*
08.910.10F	07-19	CE *
08.910.10S	07-19	CE*
08.910.11	07-20	C €*
08.910.11F	07-19	CE*
08.910.11S	07-19	CE*
08.910.12	07-20	CE*
08.910.13	07-20	CE*
08.910.13F	07-19	CE*
08.910.13S	07-19	CE*
08.910.22	07-19	CE*
08.911.30	07-20	C €*
08.912.10	07-20	CE *
08.912.50	07-20	(€*
08.912.75	07-20	(€*
08.915.02	07-35	C €*
08.915.05	07-35	C €*
08.917.00	07-35	CE
08.917.05	07-35	CE
08.917.07	07-35	CE
08.917.13	07-35	CE
08.917.20	07-35	CE
08.920.03	07-20	CE*
08.920.04	07-20	CE*
08.920.05	07-20	CE*
08.920.06	07-20	CE*
08.920.13	07-20	CE*
08.920.16	07-20	CE*
10.681.07	05-26	CE
10.681.13	05-26	CE
10.681.22	05-26	CE
10.681.29	05-26	CE
10.681.33	05-26	CE

10.681.51	05-26	CE
10.681.52	05-26	CE
10.685.07	05-32	CE
10.685.13	05-32	CE
10.685.22	05-32	CE
10.685.29	05-32	CE
10.685.33	05-32	CE
10.685.51	05-32	CE
10.685.52	05-32	CE
101.24526B	06-30	CE
12.002.00Z	05-09	CE
12.007.00Z	05-09	CE
12.013.00Z	05-10	CE
12.017.00Z	05-09	CE
12.018.00Z	05-09	CE
12.021.90Z	05-12	CE
12.022.00Z	05-11	CE
12.033.01Z	05-10	CE
12.034.00Z	05-12	CE
12.034.00Z	05-18	CE
12.034.01Z	05-12	CE
12.034.07Z	05-14	CE
12.034.08Z	05-14	CE
12.035.00Z	05-12	CE
12.035.00Z	05-18	CE
12.035.01Z	05-12	CE
12.035.07Z	05-14	C€
12.035.08Z	05-14	CE
12.036.00Z	05-13	CE
12.036.00Z	05-19	CE
12.036.01Z	05-13	CE
12.036.01Z	05-19	CE
12.036.07Z	05-14	CE
12.036.08Z	05-14	CE
12.044.15Z	05-15	CE
12.045.15Z	05-15	CE
12.045.15ZS	05-15	CE
12.045.15ZS	05-31	CE
12.045.15ZSTI	05-31	CE
12.051.01Z	05-10	CE
12.051.15Z	05-15	CE
12.051.15ZS	05-15	CE
12.051.15ZS	05-31	CE
12.051.15ZSTI	05-31	CE
12.059.00Z	05-17	CE
12.067.01Z	05-10	CE
12.067.17Z	05-09	CE
12.067.18Z	05-09	C€
12.067.90Z	05-15	CE
12.067.95Z	05-13	C€
12.067.95Z	05-19	CE
12.073.01Z	05-10	CE

12.079.00Z	05-11	CE
12.079.90Z	05-15	CE
12.079.95Z	05-13	CE
12.079.95Z	05-19	CE
12.087.00Z	05-11	CE
12.213.00Z	05-30	CE
12.213.00ZD	05-30	CE
12.213.00ZD	05-30	CE
		CE
12.217.00Z	05-31	
12.217.00ZD	05-31	CE
12.217.00ZTI	05-31	CE
12.218.00Z	05-31	CE
12.218.00ZD	05-31	CE
12.218.00ZTI	05-31	CE
12.221.90Z	05-31	CE
12.221.90ZD	05-31	CE
12.221.90ZTI	05-31	CE
12.222.00Z	05-31	CE
12.222.00ZD	05-31	CE
12.222.00ZTI	05-31	CE
12.234.07Z	05-30	C€
12.234.07ZD	05-30	CE
12.234.07ZTI	05-30	CE
12.234.08Z	05-30	C€
12.234.08ZD	05-30	C€
12.234.08ZTI	05-30	C€
12.235.07Z	05-30	CE
12.235.07ZD	05-30	CE
12.235.07ZTI	05-30	CE
12.235.08Z	05-31	CE
12.235.08ZD	05-31	C€
12.235.08ZTI	05-31	CE
12.236.07Z	05-30	CE
12.236.07ZD	05-30	CE
12.236.07ZTI	05-30	CE
12.236.08Z	05-30	C€
12.236.08ZD	05-30	CE
12.236.08ZTI	05-30	CE
12.267.01Z	05-31	CE
12.267.01ZD	05-31	CE
12.267.01ZTI	05-31	CE
12.279.90Z	05-30	CE
12.279.90ZD	05-30	CE
12.279.90ZTI	05-30	CE
12.300.08	05-00	CE
12.300.08	05-01	CE
12.300.11	05-04	CE
12.300.11	05-03	CE
12.300.15	05-04	CE
12.300.16	05-04	CE
12.300.17	05-04	CE
12.300.20	05-04	CE



Numerical Index 11-09

12.300.30	05-05	C€
12.300.35	05-05	CE
12.300.45	05-03	CE
12.300.45	05-05	CE
12.300.47	05-05	CE
12.300.60	05-05	CE
12.300.65	05-05	CE
12.300.70	05-05	CE
12.300.75	05-05	CE
12.300.80	05-05	CE
12.302.00	05-02	CE
12.302.00	05-03	CE
12.302.00	05-04	CE
12.302.01	05-04	CE
12.303.00	05-02	CE
12.303.00	05-02	CE
12.303.00	05-03	CE
12.522.15Z	05-16	CE
12.522.16Z	05-16	CE
12.701.00Z	05-18	CE
14.001.00	05-18	CE
14.001.01	05-20	CE
14.010.09	05-20	CE
14.010.11	05-25	CE
14.016.00	05-21	CE
14.017.00	05-21	CE
14.018.15	05-21	()
14.018.16	05-20	()
14.023.00	05-20	()
14.053.15	05-21	CE
14.053.16	05-21	()
14.065.00	05-22	(E
14.069.00	05-22	CE
14.088.15	05-22	CE
14.088.16	05-22	€
14.101.00	05-22	€
14.150.00	05-23	€
14.150.00D	05-23	€
14.150.05	05-23	€
14.150.10	05-24	CE
14.150.11	05-24	CE
14.151.00	05-23	CE
14.151.00D	05-23	CE
14.151.01	05-23	€
14.151.05	05-23	CE
14.151.10	05-25	CE
14.151.11	05-24	CE
14.210.05	05-24	CE
14.217.00	05-24	CE
14.222.00	05-25	CE
14.222.11	05-25	CE
14.700.01	05-16	CE

14.700.01Z	05-16	CE
14.700.10Z	05-17	CE
14.701.10Z	05-17	CE
15.021.90	05-35	CE
15.034.00	05-34	CE
15.034.01	05-34	CE
15.035.00	05-34	CE
15.035.01	05-34	CE
15.036.00	05-35	CE
15.036.01	05-35	CE
15.045.15	05-35	CE
15.051.15	05-35	CE
15.067.90	05-34	CE
15.079.90	05-35	CE
15.213.00	05-39	CE
15.213.00D	05-39	CE
15.217.00	05-39	CE
15.217.00D	05-39	CE
15.218.00	05-39	CE
15.218.00D	05-39	CE
15.222.00	05-39	CE
15.222.00D	05-39	CE
15.234.07	05-39	CE
15.234.07 15.234.07D		
	05-38	CE
15.234.08	05-38	CE
15.234.08D	05-38	CE
15.235.07	05-38	CE
15.235.07D	05-38	CE
15.235.08	05-38	CE
15.235.08D	05-38	CE
15.236.07	05-39	CE
15.236.07D	05-39	CE
15.236.08	05-39	CE
15.236.08D	05-39	CE
15.267.01	05-39	CE
15.267.01D	05-39	CE
15.279.90	05-39	CE
15.279.90D	05-39	CE
17.001.00	05-52	CE
17.001.01	05-52	CE
17.001.02	05-52	CE
17.001.03	05-52	CE
17.001.10	05-52	CE
17.001.11	05-52	CE
17.001.12	05-52	CE
17.001.13	05-52	CE
17.006.01	05-57	CE
17.006.02	05-57	CE
17.006.03	05-57	CE
17.006.04	05-57	CE
17.007.00	05-48	CE
17.007.01	05-42	CE
	-1	

17.007.01	05-48	CE
17.007.01TI	05-42	CE
17.007.02	05-42	CE
17.007.02	05-48	CE
17.007.02TI	05-42	CE
17.007.03	05-42	CE
17.007.03	05-48	CE
17.007.03TI	05-42	CE
17.007.04	05-43	CE
17.007.04	05-48	CE
17.007.04TI	05-43	CE
17.007.05	05-43	CE
17.007.05	05-48	CE
17.007.05TI	05-43	CE
17.007.06	05-43	CE CC
17.007.06TI	05-43	CE CC
17.007.07	05-43	(E
17.007.07TI	05-43	(E
17.008.01	05-43	CE
17.008.01TI	05-43	CE
17.008.02	05-44	CE
17.008.02TI	05-44	CE
17.008.03	05-44	CE
17.008.03TI	05-44	CE
17.008.04	05-44	CE
17.008.04TI	05-44	CE
17.008.05	05-44	C€
17.008.05TI	05-44	CE
17.008.06	05-44	CE
17.008.06TI	05-44	CE
17.008.08	05-45	CE
17.008.08TI	05-45	C€
17.008.09	05-45	CE
17.008.09TI	05-45	CE
17.008.10	05-45	CE
17.008.10TI	05-45	C€
17.008.11	05-45	CE
17.008.11TI	05-45	CE
17.008.90	05-45	CE
17.008.90TI	05-45	CE
17.009.01	05-47	C€
17.009.02	05-47	CE
17.009.05	05-47	C€
17.010.02	05-56	CE
17.010.03	05-56	CE
17.013.00	05-52	CE
17.013.01	05-52	CE
17.013.02	05-52	CE
17.014.00	05-58	CE
17.014.01	05-58	CE
17.014.02	05-58	CE
17.020.01	05-58	CE
	00-00	~~



¹¹⁻¹⁰ Numerical Index

+49(0)7464/98880

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

47.000.00	05 50	
17.020.02	05-58	CE
17.045.00	05-50	CE
17.045.04	05-50	CE
17.045.05	05-50	CE
17.051.01	05-54	CE
17.051.02	05-54	CE
17.051.03	05-54	CE
17.052.01	05-54	CE
17.052.02	05-54	CE
17.052.03	05-54	C€
17.053.02	05-54	CE
17.053.03	05-54	CE
17.055.01	05-54	C€
17.055.02	05-54	CE
17.055.03	05-54	CE
17.056.01	05-54	CE
17.056.02	05-54	CE
17.056.03	05-54	CE
17.100.08	05-57	CE
17.100.09	05-57	CE
17.100.10	05-57	CE
17.100.11	05-57	CE
17.100.35	05-56	CE
17.100.39	05-61	CE
17.100.40	05-61	CE
17.100.46	05-56	CE
17.100.57	05-56	CE
17.100.60	05-56	CE
17.100.61	05-56	CE
17.100.62	05-56	CE
17.101.60	05-56	CE
17.101.61	05-56	CE
17.101.62	05-56	CE
17.195.00	05-55	CE
17.200.01	05-53	CE
17.200.02	05-53	CE
17.200.02	05-53	CE
17.201.01	05-53	CE
17.201.02	05-53	
17.301.00		CE
17.301.00	05-59	CE CE
	05-59	
17.303.00	05-59	CE
17.304.00	05-59	CE
17.336.15	05-61	CE
17.336.16	05-61	CE
17.337.15	05-61	CE
17.337.16	05-61	()
17.395.01	05-55	€
17.395.02	05-55	€
17.395.03	05-55	€
17.396.01	05-55	€
17.396.02	05-55	CE

17.396.03	05-55	C€
17.410.03	05-58	CE
17.677.16	05-59	CE
17.677.17	05-59	C€
17.700.00	07-12	C€
17.700.40	07-12	C€
17.700.45	07-12	C€
17.710.00	07-16	C€
19.010.00	04-21	C€
19.015.00	04-21	CE
19.015.50	04-21	CE
19.037.01	04-21	CE
19.060.00	04-24	CE
19.061.01	04-24	CE
19.061.02	04-24	CE
19.061.03	04-24	C€
19.061.13	04-24	CE
19.062.00	04-24	CE
19.063.01	04-24	CE
19.099.00	04-23	C€
19.125.00	04-21	CE
19.199.00	04-22	CE
19.200.00	04-04	CE
19.200.30	04-05	CE
19.201.11	04-04	CE
19.201.21	04-04	CE
19.201.31	04-04	CE
19.202.00	04-01	CE
19.202.00	04-04	CE
19.270.50	06-11	C€
19.272.00	09-04	C€
19.272.01	09-04	C€
19.272.02	09-04	C€
19.272.03	09-04	CE
19.272.10	09-04	CE
19.273.00	09-04	C€
19.274.00	09-03	CE
19.274.01	09-03	C€
19.274.13	09-03	C€
19.274.50	09-03	C€
19.274.60	09-03	CE
19.275.00	09-04	C€
19.275.01	09-04	CE
19.275.02	09-04	C€
19.275.04	09-04	C€
19.277.01Z	09-01	C€
19.279.00	09-05	C€
19.281.15TC	04-27	CE
19.281.15TC	09-02	C€
19.281.16	09-05	C€
19.509.10	03-37	C€
19.509.20	03-37	C€

19.512.03	03-39	CE
19.512.04	03-39	CE
19.512.06	03-39	CE
19.512.09	03-39	CE
19.512.13	03-39	CE
19.512.14	03-39	CE
19.512.14	03-39	CE
		CE
19.512.19	03-39	
19.513.03	03-38	CE
19.513.04	03-38	CE
19.513.05	03-38	CE
19.516.00	03-38	CE
19.521.00	03-38	CE
19.561.13	03-36	CE
19.574.14	06-42	C€
19.574.16	06-42	CE
19.576.13	06-42	CE
19.576.14	06-42	C€
19.576.16	06-42	CE
19.600.18	06-42	CE
19.600.25	06-42	CE
19.641.02	06-41	CE
19.641.03	06-41	CE
19.649.15	06-40	CE
19.649.30	06-40	CE
19.649.50	06-40	CE
19.649.60	03-36	CE
19.651.13	06-40	CE
19.651.13	07-29	CE
19.651.14		CE
	06-40	
19.651.14	07-29	CE
19.651.15	06-40	CE
19.651.15M	06-40	CE
19.651.15M	07-27	CE
19.651.30	06-40	CE
19.700.00	06-41	CE
19.700.05	06-41	CE
19.710.18	06-41	CE
19.714.01	07-34	C€
19.714.02	07-34	CE
19.714.03	07-34	C€
19.714.04	07-34	CE
19.714.16	07-34	CE
19.750.00	06-41	CE
19.762.00	06-41	CE
22.011.03	02-08	CE
22.014.03	02-08	CE
22.024.03	02-09	CE
22.024.04	02-09	CE
22.025.03	02-09	CE
22.025.03	07-04	CE
22.025.03	08-13	CE
22.023.03	00-10	



Numerical Index 11-11

h.

22.025.03D	02-09	C€
22.031.08	03-36	CE
22.051.03	02-08	CE
22.100.15	04-24	CE
22.101.15	04-24	CE
22.106.01	06-02	CE
22.107.21	03-36	CE
22.200.12	06-02	CE
22.200.13	06-02	CE
22.200.14	06-02	CE
22.200.15	06-02	CE
22.200.20	06-02	CE
22.230.13	06-02	CE
22.230.14	06-02	CE
22.270.12	06-05	CE
22.272.15	06-04	CE
22.278.12	06-02	CE
22.278.15	06-02	CE
22.279.15	06-02	CE
22.281.15TC	04-27	CE
22.310.12	06-05	CE
22.310.15	06-05	CE
22.400.13	06-03	CE
22.400.14	06-03	CE
22.408.11	06-03	CE
22.408.13	06-03	CE
22.408.14	06-03	CE
22.408.16	06-03	CE
22.408.20	06-03	CE
22.416.15	06-05	CE
22.430.17	06-05	CE
22.450.18	06-05	CE
22.480.12	06-03	CE
22.480.15	06-03	CE
22.481.12	06-03	CE
22.481.15	06-03	CE
22.486.12	06-05	CE
22.486.15	06-05	CE
22.488.12	06-04	CE
22.488.15	06-04	CE
22.488.20	06-05	CE
22.489.00	06-04	CE
22.489.00	07-04	CE
22.489.00M	06-04	CE
22.489.00M	08-13	CE
22.489.01	06-04	CE
22.523.13	03-37	CE
22.523.13	03-37	CE
22.523.13 22.523.90D	03-37	CE
22.523.90D 22.523.90D	03-37	CE
22.810.17	04-27	CE
22.810.17	08-13	CE
22.010.17	00-13	ce

22.810.17	08-15	CE
22.810.17D	08-09	CE
22.811.17	08-09	CE
22.811.17D	08-09	CE
22.812.17	08-10	CE
22.814.17	08-10	C€
22.815.17	08-09	C€
22.816.17	08-09	CE
22.820.17	08-10	CE
22.820.17D	08-10	C€
22.820.17TC	08-10	C€
22.821.17	08-10	CE
22.821.17D	08-10	C€
22.824.17	06-03	CE
22.830.17	08-04	CE
23.050.10	06-07	CE
23.051.10	06-07	CE
23.054.12	06-07	CE
23.055.12	06-07	CE
23.058.12	06-07	CE
23.059.12	06-07	CE
23.060.12	06-07	CE
23.061.12	06-07	CE
23.062.12	06-07	CE
23.063.12	06-07	CE
23.098.14	06-06	CE
23.099.14	06-06	CE
23.104.14	06-07	CE
23.105.14	06-07	CE
23.105.50	06-46	CE
23.106.14	06-07	CE
23.106.16	06-07	CE
23.106.18	06-07	CE
23.107.14	06-07	CE
23.107.16	06-07	CE
23.107.18	06-07	CE
23.120.12	04-26	CE
23.705.09	06-07	CE
23.709.11	06-06	CE
23.740.20	06-06	CE
23.741.20	06-06	CE
23.781.15	06-06	CE
23.782.15	06-06	CE
24.058.01	06-45	CE
24.058.02	06-45	CE
24.058.03	06-45	CE
24.058.04	06-45	CE
24.058.10	06-45	CE
24.061.22	02-04	CE
24.061.24	02-04	CE
24.062.24	02-04	CE
24.062.24	02-04	CE
L-T.VVL.L.T.	02-04	

24.062.30	02-06	CE
24.062.31	02-06	CE
24.067.22	02-04	C€
24.067.24	02-04	CE
24.070.22	02-04	CE
24.070.24	02-04	C€
24.071.22	02-04	CE
24.071.24	02-04	CE
24.072.22	02-04	CE
24.072.22.	07-03	CE
24.074.13	03-37	CE
24.074.15	03-37	CE
24.074.16	03-37	
24.074.17	03-37	CE
24.075.22	02-04	CE
24.075.24	02-04	CE
24.080.01	02-03	
24.086.01	02-03	CE
24.087.00		CE
	02-03	
24.087.02 24.089.02	08-13	CE CC
	02-03	
24.089.02	06-08	CE
24.098.03A	07-03	CE
24.099.08	02-05	CE
24.099.09	02-05	
24.099.17	02-05	CE
24.099.23	02-05	CE
24.099.25	02-05	CE
24.101.08	02-10	
24.101.09	02-10	CE
24.101.17	02-10	CE
24.101.23	02-10	CE
24.102.03A	02-10	CE
24.102.08	02-10	CE
24.102.09	02-10	CE
24.102.17	02-10	CE
24.102.23	02-10	CE
24.112.05	02-10	CE
24.114.00	08-13	€
24.124.06	02-10	CE
24.201.01G	03-16	CE
24.201.01GM5	03-13	CE
24.201.01GM5OX	03-06	CE
24.201.01GM5-TI	03-21	CE
24.201.05L	03-14	CE
24.201.05L	03-19	CE
24.201.05L	08-12	CE
24.201.05L-TI	03-20	C€
24.202.03G	03-16	C€
24.203.05G	03-12	CE
24.203.05G	03-15	CE
24.203.05G	03-16	C€



All CE marked products according to the Medical Device Directive 93/42/EEC K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻¹² Numerical Index

+49(0)7464/98880

24.204.11G	03-12	CE
24.204.11G	03-15	CE
24.204.11G	03-17	CE
24.204.11GM5	03-13	C€
24.204.11GM5OX	03-06	C€
24.204.11GM5-TI	03-21	CE
24.204.15G	03-17	CE
24.205.06HF	07-03	CE
24.205.07G	03-12	CE
24.205.07G	03-15	CE
24.205.07G	03-16	CE
24.205.07GM5	03-13	CE
24.205.07GM5OX	03-06	CE
24.205.07GM5-TI	03-21	CE
24.206.09G	03-16	CE
24.207.02C	03-18	CE
24.207.02C	03-18	CE
24.207.04C 24.207.04C-TI		CE
	03-20	
24.207.06HF	07-03	€
24.207.13C	03-18	CE
24.207.13G	03-12	CE
24.207.13G	03-15	CE
24.207.13G	03-17	CE
24.207.13GM5	03-13	CE
24.207.13GM5OX	03-06	CE
24.207.13GM5-TI	03-21	CE
24.207.13MC	03-18	CE
24.207.17G	03-17	C€
24.207.17MC	03-19	C€
24.207.23	03-14	CE
24.207.23	03-19	CE
24.208.02CI	03-22	C€
24.208.02T	03-23	CE
24.208.03L	03-14	CE
24.208.03L	03-19	CE
24.208.03L	08-12	CE
24.208.03L-TI	03-20	CE
24.208.04S	03-12	CE
24.208.04S	03-13	CE
24.208.04S	03-14	CE
24.208.04S	03-15	CE
24.208.04S	03-23	CE
24.208.04SD	03-23	CE
24.208.04SDOX	03-07	CE
24.208.04SOX	03-06	CE
24.208.06H	03-15	CE
24.208.06H	03-22	CE
24.208.06HF	03-22	CE
24.208.23A	03-23	CE
24.208.23AOX	03-07	CE
24.208.30S	03-07	CE
24.208.35U	03-22	C€

24.209.04GX	03-23	CE
24.210.01L	03-14	CE
24.210.01L	03-19	CE
24.210.01L	08-12	CE
24.210.01L-TI	03-20	CE
24.221.01GM5OX	03-06	CE
24.224.11GM5OX	03-06	CE
24.225.07GM5OX	03-06	C€
24.227.13GM5OX	03-06	CE
24.228.04SOX	03-06	CE
24.228.04SOX	03-07	CE
24.228.23AOX	03-07	CE
24.353.02	09-07	ce
24.437.01	03-28	CE
24.437.02	03-28	CE
24.437.03	03-29	CE
24.437.04	03-29	CE
24.437.07	03-29	CE
24.451.00	03-08	CE
24.451.01	03-08	CE
24.451.02	03-08	CE
24.451.02	03-09	CE
24.451.03	03-08	CE
24.451.06	03-08	CE
24.453.03	03-10	CE
24.453.12	03-10	CE
24.453.15	03-09	CE
24.453.22	03-10	CE
24.453.23	03-10	CE
24.454.01	03-11	CE
24.454.01	03-15	CE
24.454.02	03-11	CE
24.454.03	03-09	CE
24.454.03	03-11	CE
24.454.05	03-11	CE
24.454.06	03-11	CE
24.454.06TI	03-11	CE
24.455.06	03-09	CE
24.455.06	07-03	CE
24.488.01	03-28	CE
24.488.02	03-28	CE
24.490.01	03-30	CE
24.490.02	03-30	CE
24.491.01	03-31	CE
24.491.02	03-31	CE
24.493.01	03-30	CE
24.493.02	03-30	CE
24.493.03	03-30	CE
24.494.00	03-31	CE
24.495.01	03-31	CE
24.495.01	07-11	CE
24.495.02	03-31	CE
-		· · ·

24.495.02	07-11	CE
24.495.03	03-31	CE
24.495.03	07-11	CE
24.548.01	06-42	CE
24.551.01	03-24	CE
24.551.03	03-24	CE
24.551.05	03-24	CE
24.551.07	03-24	CE
24.551.09	03-24	CE
24.551.11	03-25	CE
24.551.13	03-25	CE
24.551.15	03-25	CE
		CE
24.551.17	03-25	
24.551.24S	03-27	CE
24.553.01	03-26	CE
24.553.03	03-26	CE
24.553.05	03-26	CE
24.561.67	03-27	CE
24.565.33	03-27	CE
24.708.25	04-12	CE
24.708.27	04-12	CE
24.708.29	04-12	CE
24.708.31	04-12	CE
24.709.35	04-13	CE
24.709.39	04-13	CE
24.709.41	04-13	CE
24.709.45	04-13	CE
24.710.01OX	04-06	CE
24.710.02OX	04-06	C€
24.711.43	04-12	C€
24.711.44	04-12	C€
24.711.45	04-12	CE
24.725.00	03-34	CE
24.725.05	03-34	CE
24.725.07	03-34	C€
24.725.08	03-34	C€
24.725.09	03-34	C€
24.725.20	03-34	C€
24.725.21	03-35	CE
24.725.58	03-35	C€
24.725.70	03-35	CE
24.725.71	03-35	CE
24.725.72	03-35	CE
24.725.73	03-35	CE
24.725.74	03-35	CE
24.725.86	03-35	CE
24.733.18	04-13	CE
24.733.19	04-13	CE
24.733.20	04-13	CE
24.747.03	07-31	CE
24.747.04	08-13	CE
24.747.06	08-13	CE
	00 10	



K2019-03/1-E CE All CE marked products according to the Medical Device Directive 93/42/EEC are mentioned in the index from page 11-07.

zepf-dental.com

Numerical Index 11-13

24.751.101G	03-16	CE
24.751.101GM5	03-13	CE
24.751.101GM5OX	03-06	CE
24.751.101GM5-TI	03-21	CE
24.751.101L	03-14	CE
24.751.101L	03-19	CE
24.751.101L-TI	03-20	CE
24.751.102CI	03-22	CE
24.751.102G	03-16	CE
24.751.102GM5	03-13	CE
24.751.102GM5OX	03-06	CE
24.751.102GM5-TI	03-21	CE
24.751.102L	03-14	CE
24.751.102L	03-19	CE
24.751.102LC	03-18	CE
24.751.102L-TI	03-20	CE
24.751.102RC	03-18	CE
24.751.102TA	03-23	CE
24.751.103Cl	03-22	CE
24.751.103G	03-16	CE
24.751.103L	03-14	CE
24.751.103L	03-19	CE
24.751.103L-TI	03-20	CE
24.751.103TA	03-23	CE
24.751.104	03-34	CE
24.751.104G	03-16	CE
24.751.104L	03-14	CE
24.751.104L	03-19	CE
24.751.104LC	03-18	CE
24.751.104LC-TI	03-20	CE
24.751.104L-TI	03-20	CE
24.751.104RC	03-18	CE
24.751.104RC-TI	03-20	CE
24.751.104XL	03-23	CE
24.751.104XR	03-23	CE
24.751.105	03-34	CE
24.751.105G	03-12	CE
24.751.105G	03-15	CE
24.751.105G	03-16	CE
24.751.105L	03-14	CE
24.751.105L	03-19	CE
24.751.105L-TI	03-20	CE
24.751.106G	03-12	CE
24.751.106G	03-15	CE
24.751.106G	03-16	CE
24.751.106H	03-15	CE
24.751.106H	03-22	CE
24.751.106HF	03-22	CE
24.751.106HF	07-03	CE
24.751.106L	03-14	CE
24.751.106L	03-14	CE
24.751.106L-TI	03-20	CE
	00-20	~~

24.751.107G	03-12	CE
24.751.107G	03-15	CE
24.751.107G	03-16	CE
24.751.107GM5	03-13	CE
24.751.107GM5OX	03-06	CE
24.751.107GM5-TI	03-21	CE
24.751.107H	03-15	C€
24.751.107H	03-22	CE
24.751.107HF	03-22	CE
24.751.107HF	07-03	C€
24.751.108	03-35	CE
24.751.108G	03-12	CE
24.751.108G	03-15	CE
24.751.108G	03-16	CE
24.751.108GM5	03-13	CE
24.751.108GM5OX	03-06	CE
24.751.108GM5-TI	03-21	CE
24.751.109	03-35	CE
24.751.109G	03-16	CE
24.751.110	03-34	CE
24.751.110G	03-16	CE
24.751.111	03-34	CE
24.751.111G	03-12	CE
24.751.111G	03-15	CE
24.751.111G	03-17	CE
24.751.111GM5	03-13	CE
24.751.111GM5OX	03-06	CE
24.751.112G	03-12	C€
24.751.112G	03-15	CE
24.751.112G	03-17	CE
24.751.112GM5	03-13	CE
24.751.112GM5OX	03-06	CE
24.751.112L	03-34	CE
24.751.112R	03-34	CE
24.751.113C	03-18	CE
24.751.113C	03-34	CE
24.751.113G	03-12	CE
24.751.113G	03-15	CE
24.751.113G	03-17	CE
24.751.113GM5	03-13	CE
24.751.113GM5OX	03-06	CE
24.751.113GM5-TI	03-21	CE
24.751.113L	03-34	CE
24.751.113MC	03-18	CE
24.751.113R	03-34	CE
24.751.114C	03-18	CE
24.751.114C	03-34	CE
24.751.114G	03-12	CE
24.751.114G	03-15	CE
24.751.114G	03-17	CE
24.751.114GM5 24.751.114GM5OX	03-13 03-06	C€ C€

24.751.114GM5-TI	03-21	CE
24.751.114MC	03-18	CE
24.751.115G	03-17	CE
24.751.116G	03-17	C€
24.751.117MC	03-19	C€
24.751.118G	03-17	C€
24.751.118MC	03-19	C€
24.751.123AL	03-23	CE
24.751.123AR	03-23	CE
24.751.123L	03-14	CE
24.751.123L	03-19	CE
24.751.123R	03-14	CE
24.751.123R	03-19	CE
24.751.126	07-02	CE
24.751.130	03-22	CE
24.751.131	03-22	CE
24.751.135UL	03-22	CE
24.751.135UR	03-22	CE
24.751.148	03-35	CE
24.751.149	03-35	CE
24.751.150	07-02	CE
24.751.153	03-35	CE
24.751.155	07-03	CE
24.751.156	07-03	CE
24.751.167	03-35	CE
24.751.168	03-35	CE
24.751.169	03-35	CE
24.751.169	03-35	CE
24.751.170	03-35	CE
24.751.171	03-35	CE
24.751.172	03-35	CE
24.751.172	03-35	CE
24.751.172	03-35	CE
24.751.173	03-35	CE
24.751.176 S	07-02	CE
24.751.177	07-02	CE
24.751.178	07-02	CE
24.751.179	03-35	CE
24.751.179	07-02	(E
24.751.204L	03-12	(E
24.751.204L	03-13	(E
24.751.204L 24.751.204L	03-14 03-15	< <€ <
24.751.204L	03-15	CE
24.751.204LD	03-23	CE
24.751.204LOX	03-06	CE
24.751.204LOX	03-00	CE
24.751.204LOX	03-07	CE
24.751.204E0X	03-12	CE
24.751.204R	03-12	CE
24.751.204R	03-14	CE
24.751.204R	03-15	CE
	00 10	



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻¹⁴ Numerical Index

+49(0)7464/98880

	1	
24.751.204R	03-23	CE
24.751.204RD	03-23	C€
24.751.204ROX	03-06	C€
24.751.204ROX	03-07	CE
24.751.204ROX	03-07	C€
24.751.318Ti	04-02	C€
24.751.319Ti	04-03	C€
24.751.319Ti	04-05	CE
24.751.320Ti	04-03	CE
24.751.320Ti	04-05	CE
24.751.321Ti	04-02	C€
24.751.322Ti	04-02	CE
24.751.323Ti	04-02	C€
24.751.323Ti	04-02	CE
24.751.323Ti	04-05	CE
24.751.324Ti	04-02	CE
24.751.325Ti	04-02	CE
24.751.325Ti	04-02	CE
24.751.325Ti	04-05	CE
24.751.326Ti	04-02	CE
24.751.327Ti	04-02	C€
24.751.328Ti	04-03	C€
24.751.329Ti	04-03	CE
24.751.330Ti	04-03	CE
24.751.331Ti	04-03	CE
24.751.332Ti	04-03	CE
24.751.333Ti	04-03	CE
24.751.401Ti	04-03	CE
24.751.402Ti	04-03	CE
24.751.403Ti	04-03	CE
24.751.404Ti	04-03	CE
24.751.512	07-02	CE
24.751.520W	07-02	CE
24.755.02	03-05	CE
24.755.03	03-05	CE
24.853.14	07-03	CE
24.853.24	07-03	C€
24.914.10	03-32	CE
24.914.25	03-32	C€
24.914.30	03-33	C€
24.914.35	03-33	C€
24.914.40	03-33	CE
24.914.45	03-33	C€
24.916.10	03-32	C€
24.918.15	03-33	C€
24.919.15	03-33	CE
24.923.10	03-33	C€
24.923.10	05-56	C€
24.926.10	03-32	C€
24.926.75	03-32	C€
24.950.00	03-32	C€
24.950.10	10-09	CE

24.950.12	10-09	CE
24.951.01	03-32	CE
24.961.05	07-01	C€
24.961.05	07-02	C€
24.961.06	07-01	CE
24.961.06	07-02	CE
24.967.05	08-15	CE
24.971.00	08-11	CE
24.971.00	08-12	CE
24.989.55OX	03-07	CE
24.990.35	03-15	CE
24.990.50	03-12	CE
24.990.55	03-13	CE
24.990.55OX	03-07	CE
24.990.60	03-14	CE
24.995.00	07-30	CE
24.995.01	07-28	CE
26.010.01OX	02-01	CE
26.010.02OX	02-01	CE
26.010.03OX	02-01	CE
26.010.04OX	02-01	CE
26.010.05OX	02-01	CE
26.010.06OX	02-01	CE
26.010.07OX	02-01	CE
26.010.08OX	02-01	CE
26.010.09OX	02-01	CE
26.010.10OX	02-01	CE
26.010.10OX	03-04	CE
26.120.00Ti	04-01	CE
26.120.01Ti	04-01	CE
26.120.10Ti	04-03	CE
26.120.10Ti	04-05	CE
26.120.11Ti	04-02	CE
26.120.121Ti	04-02	C€
26.120.121Ti	04-05	CE
26.120.122Ti	04-02	C€
26.120.122Ti	04-05	CE
26.120.12Ti	04-02	C€
26.120.12Ti	04-05	C€
26.120.13Ti	04-07	C€
26.120.14Ti	04-07	CE
26.120.20Ti	04-02	CE
26.120.21Ti	04-02	CE
26.120.25Ti	04-02	CE
26.120.25Ti	04-05	C€
26.120.30Ti	04-02	CE
26.120.31Ti	04-03	CE
26.120.321Ti	04-03	CE
26.120.321Ti	04-05	CE
26.120.322Ti	04-03	CE
26.120.322Ti	04-05	CE
26.120.32Ti	04-03	CE

26.120.32Ti	04-05	CE
26.120.40Ti	04-03	CE
26.120.50Ti	04-03	CE
26.120.60Ti	04-03	CE
26.120.70Ti	04-03	CE
26.122.00	04-25	CE
26.122.10	04-25	CE
26.123.01	04-25	CE
26.123.02	04-25	CE
26.130.01	04-11	CE
26.130.02	04-11	CE
26.130.03	04-11	CE
26.180.06	02-03	CE
26.180.07	03-09	CE
26.180.13	03-04	CE
26.181.01	03-04	CE
26.181.03	03-04	CE
26.181.04	02-03	CE
26.182.00	05-50	CE
26.182.01	05-50	CE
26.182.02	05-50	CE
26.182.03	05-50	CE
26.182.04	05-50	CE
26.182.11	05-51	CE
26.182.12	05-51	CE
26.182.13	05-51	CE
26.182.23	05-51	CE
26.182.24	05-51	CE
26.183.00	08-13	CE
26.191.01	02-03	CE
26.191.01	02-05	CE
26.191.02	02-03	CE
26.191.02	02-05	CE
26.191.03	02-03	CE
26.191.03	02-05	CE
26.191.04	02-03	CE
26.191.04	02-05	CE
26.193.01	03-02	C€
26.193.02	03-02	CE
26.193.03	03-02	CE
26.193.04	03-02	CE
26.193.05	03-02	CE
26.193.06	03-02	CE
26.193.07	03-02	CE
26.193.08	03-02	CE
26.193.09	03-02	CE
26.193.10	02-02	CE
26.193.10	03-02	CE
26.193.10	03-04	CE
26.193.11	03-03	CE
26.193.12	03-03	C€
26.193.13	03-03	C€
	I	L



Numerical Index 11-15

26.193.14	03-03	CE
26.193.15	03-03	CE
26.193.15	03-09	CE
26.193.16	03-03	CE
26.193.17	03-03	CE
26.193.18	03-03	CE
26.193.19	03-03	CE
26.193.20	02-02	CE
26.193.20	03-03	CE
26.193.20	03-09	CE
26.194.01	03-03	CE
26.194.02	03-03	CE
26.194.03	03-03	CE
26.194.04	03-03	CE
26.194.05	03-03	CE
26.194.05	07-03	CE
26.194.06	03-03	CE
26.194.06	03-15	CE
26.194.07	03-03	CE
26.194.07	07-03	CE
26.194.08	03-03	CE
26.194.09	03-03	CE
26.194.10	02-02	CE
26.194.10	03-03	CE
26.194.11	03-03	CE
26.194.12	03-03	CE
26.194.13	03-03	CE
26.194.14	03-03	CE
26.194.15	03-03	CE
26.194.16	03-03	CE
26.194.17	03-03	CE
26.194.18	03-03	CE
26.194.19	03-03	CE
26.194.20	02-02	CE
26.194.20	03-03	CE
26.195.01	03-02	CE
26.195.02	03-02	CE
26.195.03	03-02	CE
26.195.04	03-02	CE
26.195.05	03-02	CE
26.195.06	03-02	CE
26.195.07	03-02	CE
26.195.08	03-02	CE
26.195.09	03-02	CE
26.195.10	03-02	CE
26.200.00	04-09	CE
26.200.01	04-09	CE
26.200.02	04-09	CE
26.200.03	04-09	CE
26.200.04	04-09	CE
26.200.13	04-10	CE
26.200.17	04-08	CE
	0100	

26.200.18	04-08	CE
26.200.19	04-08	CE
26.200.35	04-10	CE
26.200.36	04-10	CE
26.200.37	04-10	CE
26.260.00	04-11	CE
26.260.01	04-11	CE
26.260.02	04-11	CE
26.426.45	04-08	CE
26.428.01	04-09	CE
26.428.02	04-09	CE
26.428.03	04-09	CE
26.428.04	04-09	CE
26.430.21	04-08	CE
26.690.01	04-00	CE
26.690.02	05-49	CE
26.690.03	05-49	CE
26.690.10	05-49	CE
28.110.01	03-49	CE
28.111.01	09-07	CE
28.114.00	09-07	CE
28.116.00		CE
28.121.00	09-07	
28.130.00	04-15	CE
28.161.13	09-07	CE
	09-07	CE CE
28.161.17	09-07	
28.601.00	04-16	CE
28.601.01 28.601.02	04-16 04-16	C€
28.601.02	04-10	CE
28.601.03	04-10	CE
28.602.01	04-10	CE
28.602.02	04-16	CE
28.602.03	04-10	CE
28.603.01	04-10	CE
28.603.02	04-10	CE
28.603.03	04-10	CE
28.604.01	04-16	CE
		CE
28.604.02 28.604.03	04-16	CE
28.606.00	04-16 04-17	CE
28.606.01		
28.606.02	04-17 04-17	CE CE
28.606.02	04-17	
28.606.04	04-17	CE CE
	04-17	
28.607.01 28.607.02		CE
28.607.02	04-17	CE
28.607.03	04-17	CE
28.608.01	04-17	CE
28.608.02	04-17	CE
28.608.03	04-17	CE
28.631.00	04-14	CE

28.631.01	04-14	C€
28.631.02	04-14	C€
28.631.03	04-14	CE
28.631.04	04-14	CE
28.632.01	04-14	CE
28.632.02	04-14	CE
28.632.03	04-14	CE
28.633.01	04-14	CE
28.633.02	04-14	CE
28.633.03	04-14	C€
28.634.01	04-14	CE
28.634.02	04-14	CE
28.634.03	04-14	C€
28.636.00	04-15	C€
28.636.01	04-15	C€
28.636.02	04-15	C€
28.636.03	04-15	CE
28.636.04	04-15	CE
28.637.01	04-15	CE
28.637.02	04-15	CE
28.637.03	04-15	CE
28.638.01	04-15	CE
28.638.02	04-15	CE
28.638.03	04-15	CE
28.640.01	04-18	CE
28.640.02	04-18	CE
28.640.03	04-18	C€
28.640.04	04-18	CE
28.640.10	04-19	CE
28.645.01	04-19	CE
28.645.02	04-19	CE
28.645.03	04-19	CE
28.645.04	04-19	C€
28.661.01	04-20	C€
28.661.02	04-20	C€
28.661.03	04-20	C€
28.662.01	04-20	C€
28.662.02	04-20	CE
28.662.03	04-20	C€
28.663.02	04-20	CE
28.663.03	04-20	CE
28.664.02	04-20	C€
28.664.03	04-20	CE
28.671.00	04-20	CE
28.672.00	04-20	C€
28.681.00	04-20	C€
28.682.00	04-20	C€
31.182.01	09-02	CE
31.184.01	09-06	C€
31.184.13	09-05	C€
31.185.00	09-06	C€
31.185.01	09-06	CE

ISU

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻¹⁶ Numerical Index

+49(0)7464/98880

31.185.02	09-05	CE
31.185.04	09-06	CE
31.185.10	09-06	CE
31.185.12	09-06	CE
31.683.00	07-39	CE
31.691.13	07-37	CE
31.692.00	07-37	CE
31.693.10	07-36	CE
31.760.11	06-43	CE
37.258.40	06-08	CE
37.258.43	06-08	CE
37.261.11	06-11	CE
37.261.14	06-11	CE
37.271.00	06-11	CE
37.351.02	06-08	CE
37.426.01	06-12	CE
37.426.02	06-12	CE
37.429.12	06-11	CE
37.429.14	06-11	CE
37.429.16	06-11	CE
37.437.15	06-09	CE
37.437.17	06-09	CE
37.438.15	06-18	CE
37.440.00	06-15	CE
37.441.01	06-13	CE
37.441.02	06-13	CE
37.443.00	06-08	CE
37.444.01	06-09	CE
37.445.01	02-05	CE
37.445.01	06-08	CE
37.446.04	06-11	CE
37.448.10	02-06	CE
37.448.20	02-06	CE
37.454.00	06-10	CE
37.454.02	06-10	CE
38.074.14	06-13	CE
38.076.16	06-13	CE
38.078.16	06-13	CE
38.426.01	06-14	CE
38.426.02	06-14	CE
38.426.03	06-14	CE
38.426.04	06-14	CE
38.426.05	06-14	CE
38.426.06	06-14	CE
38.426.07	06-14	CE
38.426.08	06-14	CE
38.426.09	06-14	CE
38.427.22	06-17	CE
38.428.02	06-16	CE
38.428.03	06-16	CE
38.428.04	06-16	CE
38.428.05	06-16	CE
		·

38.428.06	06-16	CE
38.428.22	06-16	CE
38.430.03	06-15	CE
38.430.04	06-15	C€
38.430.05	06-15	C€
38.430.06	06-15	C€
38.438.04	06-17	C€
38.438.05	06-17	CE
38.438.06	06-17	CE
38.448.50	06-18	CE
38.452.00	06-12	CE
38.465.15	06-12	CE
38.467.08	06-12	C€
38.467.10	06-12	C€
38.471.15	06-13	CE
38.473.15	06-13	CE
41.010.17TC	08-08	CE
41.010.17TC-M	08-07	CE
41.011.17TC	08-08	CE
41.015.17	08-08	CE
41.015.17	08-12	CE
41.017.17	08-04	CE
41.200.15TC	08-07	CE
41.200.17TC	07-04	CE
41.200.17TC	08-07	CE
41.200.17TC	08-07	CE
41.200.17TC-K	08-06	CE
41.200.17TC-K	08-15	CE
41.201.15TC	08-07	CE
41.201.15TC	08-07	CE
41.201.17TC	08-07	CE
41.201.17TC-K	08-06	CE
41.240.12	06-39	CE
41.246.15TC	06-38	CE
41.250.15	06-39	CE
41.252.15TC	06-39	CE
41.252.15TC	08-12	CE
41.252.18TC	06-39	CE
41.256.14	06-38	CE
41.256.16	06-38	CE
41.256.18	06-38	CE
41.258.14TC	06-38	()
41.258.16TC	06-38	CE
41.258.18TC	06-38	(E
41.262.14	06-37	(E
41.262.17	06-37	CE
41.264.14	06-37	CE
41.264.17	06-37	CE
41.310.14TC	06-37	CE
41.310.17TC	06-37	(E
41.317.17TC	06-37	(E
41.318.17TC	06-37	CE

41.352.15TC	06-39	CE
41.362.12	06-39	CE
41.368.16	06-37	CE
41.368.18	06-37	CE
41.500.17	06-47	CE
41.500.17M	06-47	CE
41.501.01	06-47	CE
41.501.01	07-10	CE
41.503.00	06-47	CE
41.503.01	05-47	CE
41.503.01	06-47	CE
41.506.17	06-47	CE
41.541.02WM	05-60	CE
41.541.03WM		CE
	05-60	
41.541.04WM	05-60	CE
41.541.05WM	05-60	CE
41.751.011LU	07-03	CE
41.751.012LU	07-03	CE
41.822.01	07-28	CE
41.822.02	07-28	CE
41.822.03	07-28	CE
41.822.04	07-28	CE
41.822.05	07-29	C€
41.822.11	07-29	CE
41.822.22	07-29	CE
41.822.33	07-29	CE
41.834.11	05-50	C€
41.845.11	06-20	CE
41.845.22	06-20	C€
41.845.33	06-20	C€
41.847.00	07-25	C€
41.847.00	07-26	C€
41.847.01	07-26	CE
41.847.02	07-26	CE
41.847.03	07-26	CE
41.847.05	07-26	C€
41.847.08	07-26	CE
41.847.09	07-26	C€
41.847.10	07-26	CE
41.848.01	07-24	CE
41.848.02	07-24	CE
41.848.03	07-24	CE
41.848.05	07-24	CE
41.848.08	07-24	CE
41.848.08	08-12	CE
41.848.51	07-23	CE
41.848.52	07-23	CE
41.848.53	07-23	CE
41.853.11	07-02	CE
41.853.21	07-02	CE
41.854.11	07-02	CE
41.854.12	07-02	CE
71.004.12	07-02	



Numerical Index 11-17

5

41.854.13	07-03	CE
41.854.21	07-02	CE
41.854.22	07-02	CE
41.854.23	07-03	CE
41.855.00Z	06-20	CE
41.855.00ZS	06-20	CE
41.855.01Z	05-48	CE
41.855.01Z	06-20	CE
41.855.01ZS	06-20	CE
41.855.02Z	06-20	CE
41.855.02ZS	06-20	CE
41.855.04Z	06-20	CE
41.855.20	07-03	CE
41.855.22	07-03	CE
41.862.11	06-21	CE
41.862.12	06-21	CE
41.862.13	06-21	CE
41.862.14	06-23	CE
41.862.21	06-23	CE
41.864.01	06-19	CE
41.864.02	06-19	CE
41.864.13	06-21	CE
41.864.13	08-15	CE
41.864.20	06-30	CE
41.864.30	06-23	CE
41.864.40	06-23	CE
41.864.50	06-23	CE
41.864.60	06-21	C€
41.868.01	07-30	CE
41.868.02	07-30	CE
41.868.03	07-30	CE
41.868.04	07-30	C€
41.868.05	07-31	CE
41.868.06	07-31	CE
41.868.07	07-23	C€
41.868.07	07-29	C€
41.868.07	07-31	CE
41.868.08	07-31	CE
41.868.08M	07-27	C€
41.868.09	07-27	CE
41.874.04	06-19	CE*
41.874.16	06-19	<€*
41.877.23	06-19	<€*
41.878.11	06-22	<€*
41.878.12	06-22	€*
41.878.13	06-22	(6*
41.878.14	06-22	€*
41.881.01	06-43	<€*
41.881.02	06-43	€*
41.905.00	06-44	€*
41.914.16	06-44	(6*
41.916.15	06-44	€*

/1 017 15	06 44	((*
41.917.15 42.315.16	06-44	CE*
	06-24	
42.315.16S 42.316.15	06-24 06-24	C€
42.320.14	06-25	C€
42.320.15 42.321.90	06-25	CE
42.321.90	06-25 06-24	CE
42.324.15	06-24	CE
42.328.15	06-24	CE
42.326.15	06-24	<u>(</u>
42.334.17	06-25	CE
42.358.15	06-25	CE
42.360.15	06-24	CE
42.362.15	06-24	CE
42.404.16	06-24	CE
42.406.14	06-26	CE
42.620.18	06-26	CE
42.621.18	06-26	CE
42.646.15	06-26	CE
42.647.15	06-26	CE
42.650.18	06-25	CE
42.652.18	06-25	CE
46.005.65	06-28	CE
46.005.70	06-29	CE
46.007.00	06-28	CE
46.007.00	08-13	CE
46.007.01	06-28	CE
46.007.02	06-27	CE
46.007.02	07-04	CE
46.007.05	06-30	CE
46.007.10	06-30	CE
46.007.20	06-30	CE
46.007.30	06-30	CE
46.007.31	06-30	CE
46.007.40	06-28	CE
46.007.45	06-28	CE
46.007.50	06-30	CE
46.010.03	06-29	CE
46.010.04	06-29	CE
46.013.00Z	06-29	CE
46.013.00Z	08-13	CE
46.013.00Z	08-14	CE
46.013.00Z	08-15	CE
46.013.05	06-29	CE
46.013.05	08-14	CE
46.013.05Z	06-29	CE
46.014.10*	06-28	CE
46.014.11*	06-28	CE
46.014.12*	06-28	CE
46.014.12D*	06-28	CE
46.014.15*	06-28	CE
	1	I

46.014.15C*	06-28	CE
46.016.03	08-14	CE
46.016.03*	06-29	C€
46.016.04	08-14	C€
46.016.04*	06-29	CE
46.016.07	08-14	CE
46.016.07*	06-29	CE
46.016.09	08-14	CE
46.016.09*	06-29	CE
46.035.00	06-30	C€
46.035.00	08-14	C€
46.035.05	06-30	CE
46.035.05	08-12	CE
46.035.05	08-14	CE
46.035.20	08-03	CE
46.036.11	07-02	C€
46.036.21	07-02	C€
46.040.00	08-02	C€
46.040.01	08-03	C€*
46.040.02	08-03	CE*
46.040.03	08-02	CE
46.040.04	08-02	CE
46.040.07	08-03	CE
46.040.08	08-03	CE
46.040.09	08-03	CE
46.040.15	07-38	CE
46.040.30	08-03	CE
46.050.11	06-32	CE
46.050.11SC	06-32	CE
46.050.11TC	06-32	CE
46.050.11TISC	06-32	€
46.051.11	06-32	CE
46.051.11SC	06-32	€€*
46.051.11TC	06-32	CE
46.051.11TISC	06-31	€
46.051.11TISC	06-32	CE
46.057.11	06-32	CE
46.057.11SC	06-32	CE
46.057.11TC 46.057.11TISC	06-32	< < €
46.057.11TISC 46.057.11TISC	06-31 06-32	CE
46.069.11	06-32	CE
46.077.16	06-33	CE*
46.077.16SC	06-34	(6*
46.077.163C	06-34	CE
46.077.16TISC	06-34	CE
46.081.16	06-32	CE
46.081.16SC	06-32	CE
46.081.16SC	07-04	CE
46.081.16SC	08-13	CE
46.081.16TISC	06-31	CE
46.081.16TISC	06-32	CE
	00-0Z	~~



All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

¹¹⁻¹⁸ Numerical Index

+49 (0) 74 64 / 98 88 0

46.111.16	06-34	CE
46.111.16SC	06-34	C€
46.121.17	06-35	CE
46.123.17	06-35	C€
46.123.17SC	06-35	C€
46.123.17TC	06-35	CE
46.123.17TISC	06-35	CE
46.200.13	06-33	CE
46.200.13SC	06-33	C€
46.200.13TC	06-33	C€
46.200.13TISC	06-33	CE
46.201.13	06-33	CE
46.201.13SC	06-33	CE
46.201.13TC	06-33	CE
46.201.13TISC	06-31	CE
46.201.13TISC	06-33	CE
46.207.13	06-33	CE
46.207.13SC	06-33	CE
46.221.12	06-35	CE
46.319.17	08-05	CE
	08-15	CE
46.319.17		
46.319.17N	08-06	CE
46.319.17TISC	08-05	CE
46.321.16	08-05	CE
46.321.16TISC	08-05	CE
46.402.13	06-36	CE
46.402.14	06-36	CE
46.404.13	06-36	CE
46.404.14	06-36	CE
46.431.14	06-34	CE
46.431.14SC	06-34	CE
46.431.14TISC	06-31	CE
46.431.14TISC	06-34	CE
46.516.14	06-35	CE
46.517.14	06-35	C€
46.640.09	06-35	CE
46.640.13	06-35	CE
46.674.10	06-36	CE
46.675.10	06-36	C€
46.685.12	06-36	C€
46.685.12	06-43	C€
46.885.12TC	06-36	C€
46.885.12TC	06-43	CE
47.099.08	07-10	CE
47.099.10	07-10	CE
47.099.20	07-10	C€
47.099.25	07-19	CE
47.099.26	07-19	CE
47.099.31	07-10	CE
47.099.32	07-10	CE
47.099.33	07-10	C€
47.099.34	07-10	CE

47.099.50	07-08	CE
47.500.31	07-18	CE
47.501.03	10-10	CE
47.502.10	07-07	CE
47.503.10	10-11	CE
47.503.20	10-11	CE
47.503.50	10-11	CE
47.503.53	10-11	CE
47.520.00	07-33	CE
47.520.01	07-33	CE
47.520.02	07-33	<€*
47.520.03	07-33	CE
47.520.22	07-19	CE
47.520.23	07-19	CE
47.520.25	07-19	CE
47.525.50	05-03	CE
47.525.50	05-05	CE
47.525.50	09-09	CE
47.525.55	05-03	CE
47.525.55	05-05	CE
47.525.55	09-09	CE
47.530.00	07-23	د ٤*
47.560.03	07-33	CE*
47.560.05	07-33	CE
47.750.03	07-12	CE
47.750.04	07-12	CE
47.750.13	07-12	CE
47.750.14	07-12	CE
47.803.02	09-09	CE*
47.830.00	09-08	CE
47.830.00	09-09	CE
47.830.01	09-09	CE
47.832.01	09-09	CE
47.832.02	09-09	CE
47.832.04	09-09	CE
47.832.05	09-09	CE
47.832.06	09-09	CE
47.832.07	09-09	CE
47.832.08	09-09	CE
47.832.09	09-09	CE
47.833.01	09-09	CE
47.833.02	09-09	CE
47.833.03	09-09	CE
47.833.04	09-09	CE
47.833.05	09-09	CE
47.833.06	09-09	CE
47.833.07	09-09	CE
47.833.08	09-09	CE
47.833.09	09-09	CE
47.847.11	07-33	CE
47.937.00	07-06	CE
47.937.01	07-00	CE
	07-07	~~

47.937.05	07-07	CE
47.937.10	07-07	C€
47.937.11	07-07	CE
47.937.12	07-07	CE
47.937.13	07-07	CE
47.937.14	07-07	CE
47.940.00	07-13	CE
47.940.01	07-13	CE
47.942.20	07-13	CE
47.942.28	07-13	CE
47.942.33	07-13	CE
47.942.38	07-13	CE
47.942.43	07-13	CE
47.943.20	07-13	CE
47.943.28	07-13	CE
47.943.33	07-13	CE
47.943.38	07-13	CE
47.943.43	07-13	CE
47.944.20	07-13	CE
47.944.28	07-13	CE
47.944.33	07-13	CE
47.944.38	07-13	CE
47.944.43	07-13	CE
47.945.20	07-13	CE
47.945.28	07-13	ce
47.945.33	07-13	CE
47.945.38	07-13	CE
47.945.43	07-13	C€
47.949.11	07-09	CE
47.949.11	07-11	CE
47.949.12	07-09	C€
47.949.12	07-11	C€
47.949.13	07-09	C€
47.949.13	07-11	CE
47.949.21	07-11	CE
47.949.22	07-11	CE
47.949.23	07-11	C€
47.949.95	07-11	CE
47.950.02	10-10	CE
47.950.03	07-07	CE
47.954.01	07-22	CE
47.954.35	07-22	CE
47.954.55	07-22	CE
47.955.00	07-21	CE
47.955.10	07-21	CE
47.957.00	07-05	CE
47.957.01	07-05	CE
47.957.10	07-05	CE
47.957.15	07-05	CE
47.958.00	07-21	(E
		C€ C€ C€



Numerical Index 11-19

47.958.04	07-21	CE
47.961.00	07-12	CE
47.961.20	07-12	CE
47.961.20	07-12	CE
47.961.28	07-12	CE
47.961.33	07-12	CE
47.961.38	07-12	CE
47.961.43	07-12	CE
47.962.20	07-12	CE
47.962.28	07-12	CE
47.962.33	07-12	CE
47.962.38	07-12	CE
47.962.43	07-12	CE
47.962.50	07-12	CE
47.963.50	07-12	CE
47.963.60	07-12	CE
47.966.00	07-33	CE
47.990.00	07-16	CE
47.990.06	07-16	CE
47.990.08	07-16	CE
47.990.10	07-16	CE
47.990.20	07-16	CE
47.990.30	07-16	CE
47.990.40	07-16	CE
47.990.50	07-16	CE
47.990.60	07-16	CE
47.990.70	07-16	CE
47.991.00	07-17	CE
47.991.10	07-17	CE
47.991.20	07-17	C€
47.991.30	07-17	C€
47.991.40	07-17	CE
47.991.50	07-17	CE
47.991.60	07-17	CE
47.991.70	07-17	CE
47.991.80	07-17	CE
48.286.08	07-37	CE
48.666.20	07-37	CE
50.226.16	06-02	CE
50.229.16	06-02	CE
53.034.19	06-06	CE
53.034.25	06-06	CE
60.150.24	06-11	CE
60.151.24	06-11	CE
85.070.01	07-20	C€
85.070.05	07-20	C€
85.070.05	07-20	C€
85.140.00	10-08	C€
85.142.10	10-08	C€
85.142.20	10-08	C€
85.145.00	10-08	CE
85.150.00	10-08	CE

	1	
85.180.00	07-13	CE
85.180.00	08-15	CE
85.180.00	10-02	CE
85.180.03	10-02	CE
85.180.04	10-02	C€
85.180.05	10-02	C€
85.180.10	10-02	C€
85.181.00	10-02	C€
85.181.03	10-03	CE
85.181.04	05-47	CE
85.181.04	10-03	CE
85.181.05	05-47	CE
85.181.05	10-03	C€
85.181.09	10-05	CE
85.182.00	10-02	CE
85.182.03	10-05	CE
85.182.04	10-05	CE
85.182.05	10-05	CE
85.182.08	10-05	CE
85.182.50	07-07	CE
85.183.40	10-08	CE
85.183.41	10-08	CE
85.183.42	10-08	CE
85.183.43	10-08	CE
85.183.44	10-08	CE
85.183.45	10-08	CE
85.183.46	10-08	CE
85.183.47	10-08	CE
85.183.48	10-08	CE
85.183.49	10-08	CE
85.190.10	07-31	CE
85.190.10	10-11	CE
85.192.50	09-09	CE
85.192.50	10-03	CE
85.194.00	10-03	CE
85.194.10	05-04	CE
85.194.50	10-03	CE
85.195.00	05-04	CE
85.195.00	05-47	CE
85.195.00	10-03	CE
85.251.00	10-09	CE
85.251.03	07-27	CE
85.251.03	07-31	CE
85.251.03	10-09	CE
85.251.04	07-19	CE
85.251.04	07-29	CE
85.251.04	07-33	CE
85.251.04	10-09	CE
85.251.04	10-11	CE
85.251.14	07-29	CE
85.252.140	06-41	CE
85.252.25	08-12	CE

85.252.25	10-09	CE
85.255.02	07-07	CE
85.255.02	07-33	CE
85.256.00	07-33	CE
85.264.350	06-41	CE
85.312.00	10-07	CE
85.312.01	10-07	CE
85.312.02	10-07	CE
85.312.03	10-07	CE
85.312.04	10-07	CE
85.312.05	10-07	CE
85.312.06	10-07	CE
85.312.07	10-07	CE
85.312.08	10-07	CE
85.312.09	10-07	CE
85.327.00	10-07	CE
85.327.10	10-07	CE
85.327.15	10-07	CE
85.327.20	10-07	CE
85.327.30	10-07	CE
85.327.50	10-07	CE
85.327.60	10-07	CE
85.327.70	10-07	CE
85.540.60	10-07	CE
85.540.65	10-10	CE
85.703.00	10-08	CE
85.903.01	10-08	CE
85.903.03	10-08	CE
85.903.04	10-08	CE
00.000.04	10-00	

All CE marked products according to the Medical Device Directive 93/42/EEC CE K2019-03/1-E are mentioned in the index from page 11-07.

11-20 Index

+49 (0) 74 64 / 98 88 0

Terms of Delivery and Payment Helmut Zepf Medizintechnik GmbH

1. Offers and order acceptance

Our offers are always subject to confirmation and without obligation. Telephone and verbal agreements and arrangements with our agents shall become legally valid only after they have been confirmed by us in writing. Deviations in the orders of the buyers relative to our terms of delivery and payment shall not be binding for us, if we have not declared our approval in writing. The subsequent correction of potential errors in offers and invoices shall be permitted for us explicitly and in every case.

2. Delivery

All our data on delivery times shall be approximate only and non-binding.

3. Calculation

The prices agreed upon are net prices plus the respective legally applicable value-added tax.

4. Warranty

Within a period of one year we shall grant warranty for defects, which are caused by manufacturing or material faults. Potential defects shall have to be indicated to the supplier in writing immediately, at the latest, however, within eight days after receipt of the delivery. In case of justified notification of defects, the supplier shall be obligated to rework or replace as chosen. Any exceeding warranty claims, in particular for damage which has not been caused to the supplied goods themselves shall be ruled out, provided no intent or gross negligence can be substantiated. Our obligation of warranty shall not apply, if the defect or modification of the goods supplied is caused by incorrect intervention of the ordering or third parties. Moreover the warranty obligation shall not apply in case of incorrect handling or excessive wear of the goods by the ordering or third parties.

5. Packaging

If the order does not define the packaging, we shall choose the packaging at our discretion.

6. Delivery / shipment

The delivery is made ex works. The goods shall be transported to the place of destination always at the costs and risk of the buyer, no matter by which route and which means of transportation is chosen. The road tolls, provided they are not paid by us in case of freight-paid fob or cif deliveries, shall be borne by the buyer. Neither do we assume any obligation for delivery in time nor for the full utilization of loading capacity of the means of transportation. Moreover, the buyer shall bear the costs of the transport insurance.

7. Payment

Our invoices shall be due for payment without deduction within thirty days after invoicing. In case of payment within eight days we grant a discount of two per cent. Repairs and interest shall be payable immediately and without deduction. Cheques and bills of exchange shall be accepted only in lieu of payment, the latter only after previous arrangement. Costs for bills of exchange and discount charges shall be borne by the ordering party. Payments shall be considered made as from the day, at which the supplier can avail himself of the invoiced amount in cash without any loss. In case of default in payment of the ordering parts we shall be permitted to charge default interest of 5 per cent above the respective basic interest rate of the European Central Bank as from the occurrence of default, and to declare due any amounts potentially deferred. Before complete payment of all invoices due including default interest, the supplier shall not be obligated to any further deliveries from a current contract. A complaint, even when justified, shall not permit the buyer to delay payment or to change the terms of payment.

8. Retention of title

Until complete redemption of all obligations from the business relationship, also of others and future businesses of the buyer with us, the goods supplied shall remain our property. For the duration of the retention of title of the seller, the buyer obligates himself to handle the goods correctly and with care. Within the framework of his normal standard business operation, the buyer may sell and process the goods. The claims of the buyer from the sales of the goods subject to retention of title shall be assigned to us now already until our claims from good delivery are paid off completely, irrespective of whether the goods subject to retention of title have been sold without or after processing or whether they have been sold to one or several buyers. The assigned claims serve as our security, however only to the value of the respectively sold goods subject to retention of title. The buyer is entitled to sell the goods subject to retention of title only in keeping with the agreement hereinbefore on the assignment of the purchase price claim. In case of seizure of the goods or the transfer of the purchase price claim to a third party in their place, the buyer is obligated to inform us immediately. We obligate ourselves to return or to transfer back the securities assigned to us at our discretion in keeping with the conditions mentioned hereinbefore, provided the value exceeds the claims to be secured by 20 per cent.

9. Place of performance and venue

The place of performance and venue shall be D-78532 Tuttlingen in Germany for all rights and obligations arising from the business relationship with us. The law of the Federal Republic of Germany shall apply exclusively for all legal matters under exclusion of the conflict of laws and the agreement of the United Nations on Contracts of the International Sale of Goods (CISG).

10. Data storage

We are permitted to save and process personal data of the ordering party.

11. Final clauses

The potential ineffectiveness of individual stipulations of these terms of business shall not affect the validity of the other stipulations.







